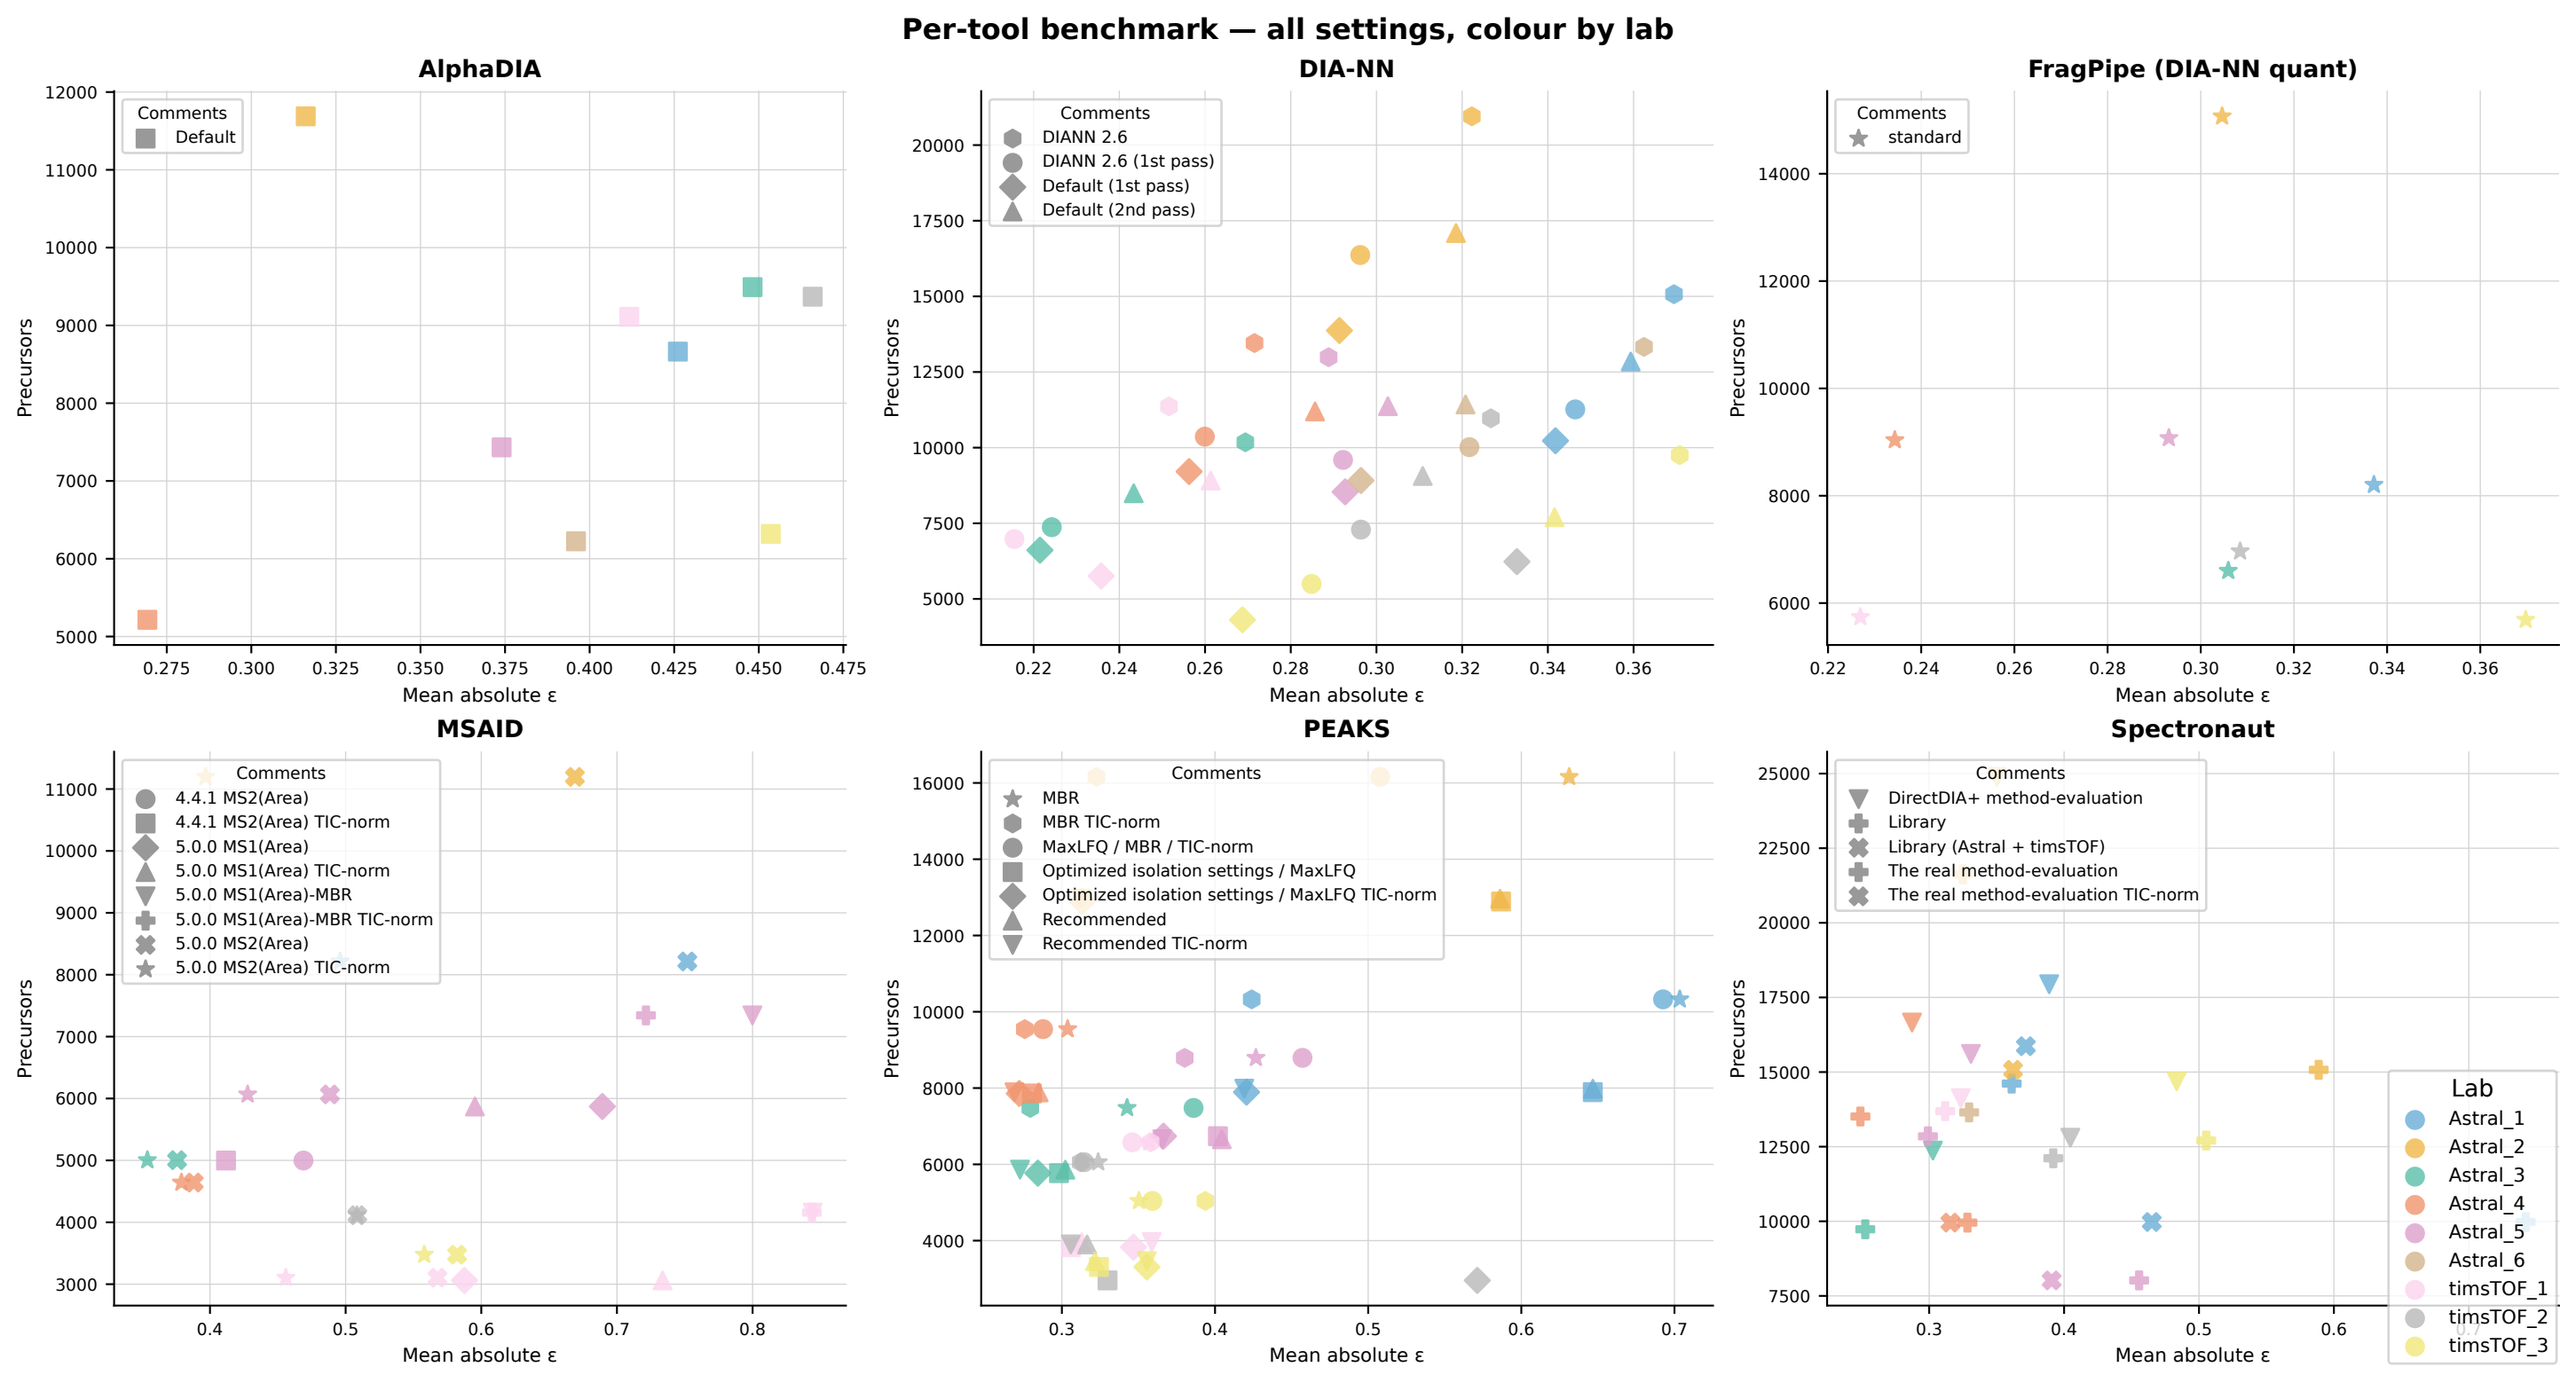
Per-tool benchmark — all settings, colour by lab
AlphaDIA
DIA-NN
FragPipe (DIA-NN quant)
MSAID
PEAKS
Spectronaut
Precursors
Mean absolute ε
Comments
Default
DIANN 2.6
DIANN 2.6 (1st pass)
Default (1st pass)
Default (2nd pass)
standard
4.4.1 MS2(Area)
4.4.1 MS2(Area) TIC-norm
5.0.0 MS1(Area)
5.0.0 MS1(Area) TIC-norm
5.0.0 MS1(Area)-MBR
5.0.0 MS1(Area)-MBR TIC-norm
5.0.0 MS2(Area)
5.0.0 MS2(Area) TIC-norm
MBR
MBR TIC-norm
MaxLFQ / MBR / TIC-norm
Optimized isolation settings / MaxLFQ
Optimized isolation settings / MaxLFQ TIC-norm
Recommended
Recommended TIC-norm
DirectDIA+ method-evaluation
Library
Library (Astral + timsTOF)
The real method-evaluation
The real method-evaluation TIC-norm
Lab
Astral_1
Astral_2
Astral_3
Astral_4
Astral_5
Astral_6
timsTOF_1
timsTOF_2
timsTOF_3