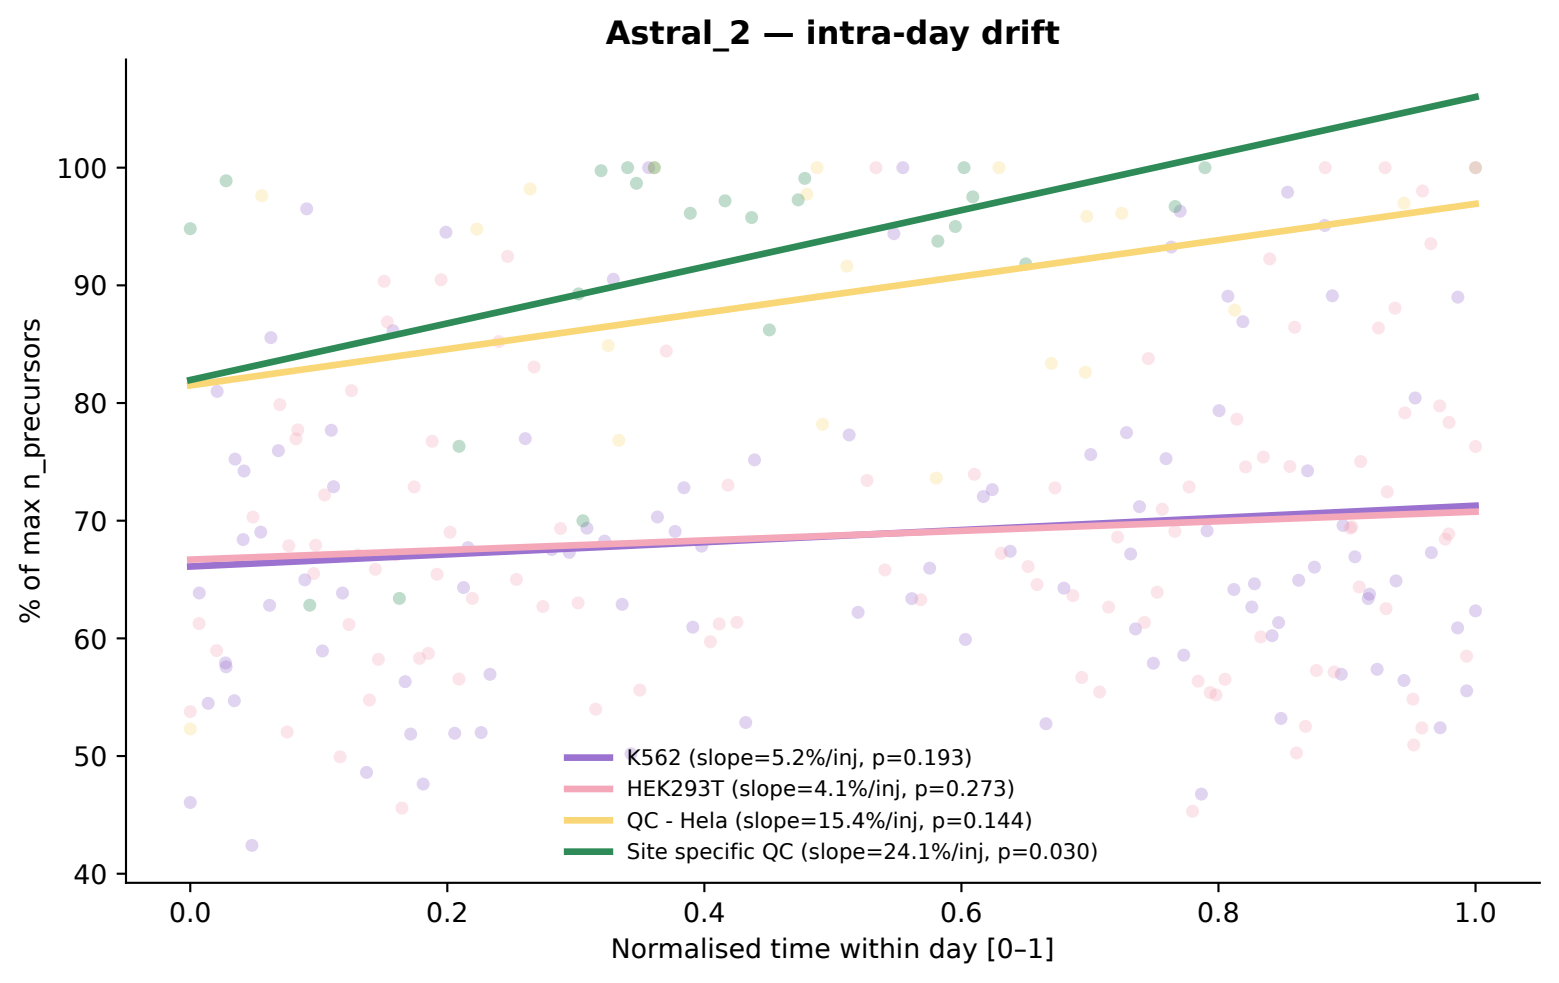
Astral_2 — intra-day drift
% of max n_precursors
Normalised time within day [0–1]
K562 (slope=5.2%/inj, p=0.193)
HEK293T (slope=4.1%/inj, p=0.273)
QC - Hela (slope=15.4%/inj, p=0.144)
Site specific QC (slope=24.1%/inj, p=0.030)