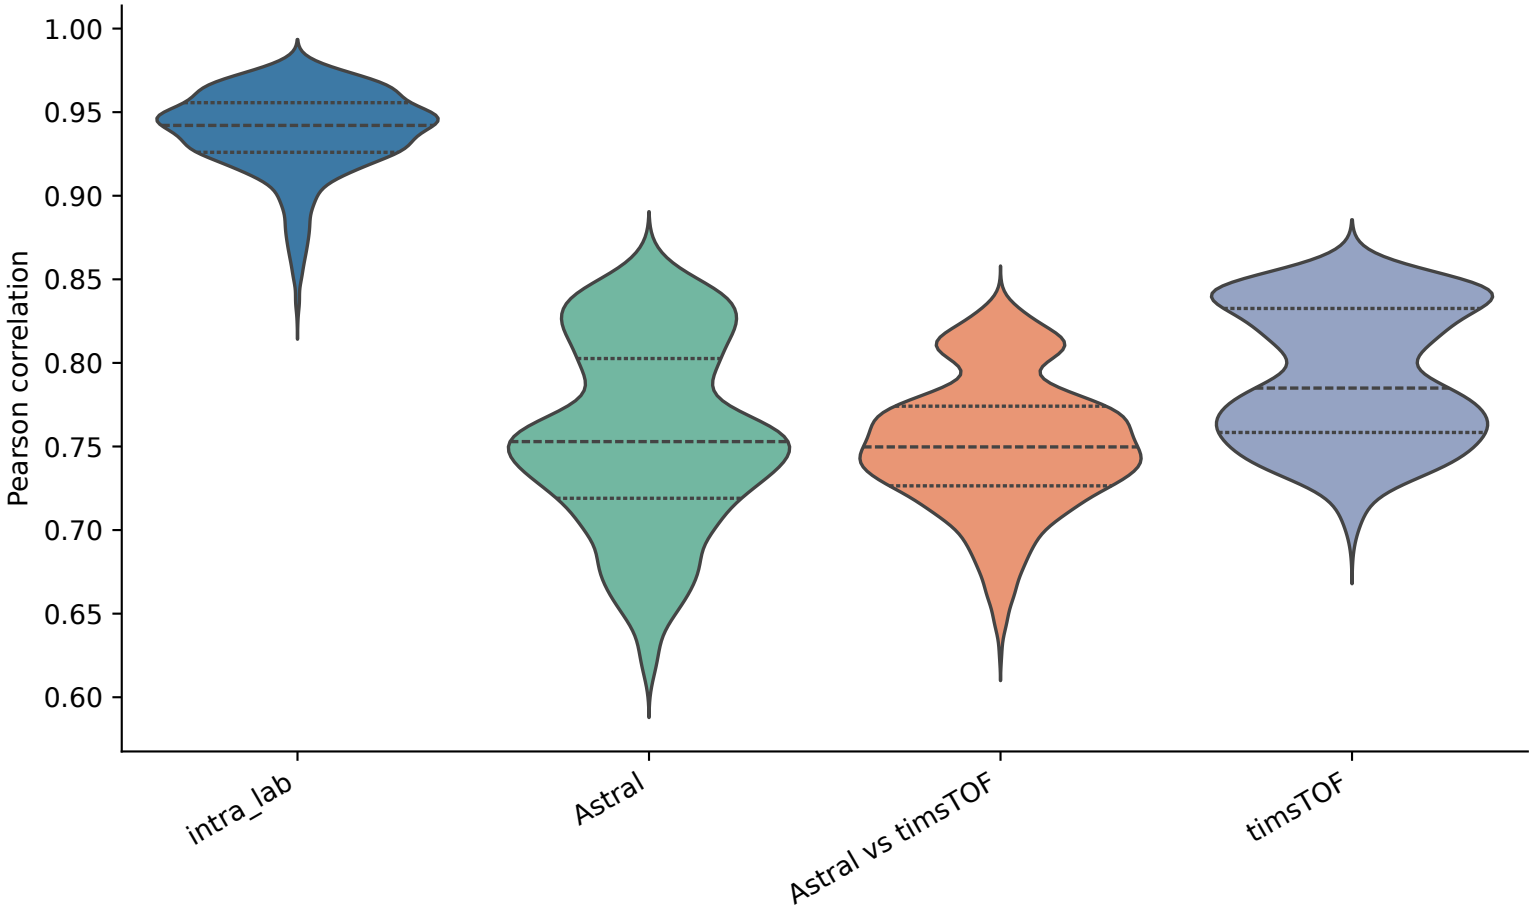
Site specific QC — correlation by instrument type
Pearson correlation
1.00
0.95
0.90
0.85
0.80
0.75
0.70
0.65
0.60
intra_lab
Astral
Astral vs timsTOF
timsTOF