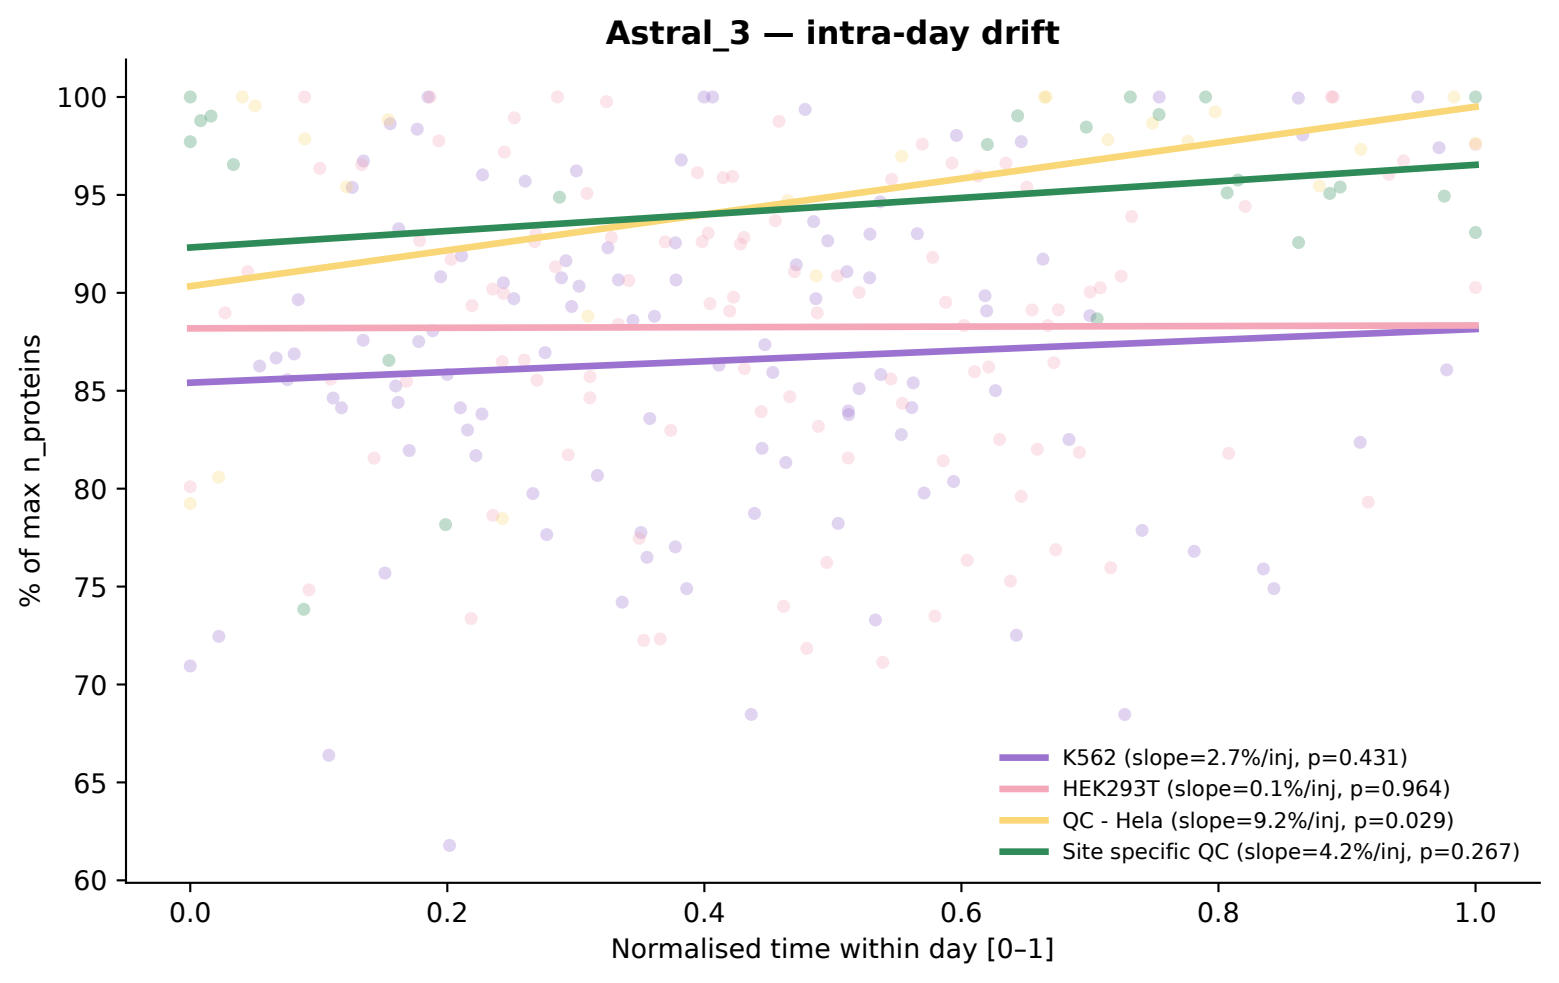
Astral_3 — intra-day drift
% of max n_proteins
Normalised time within day [0–1]
K562 (slope=2.7%/inj, p=0.431)
HEK293T (slope=0.1%/inj, p=0.964)
QC - Hela (slope=9.2%/inj, p=0.029)
Site specific QC (slope=4.2%/inj, p=0.267)