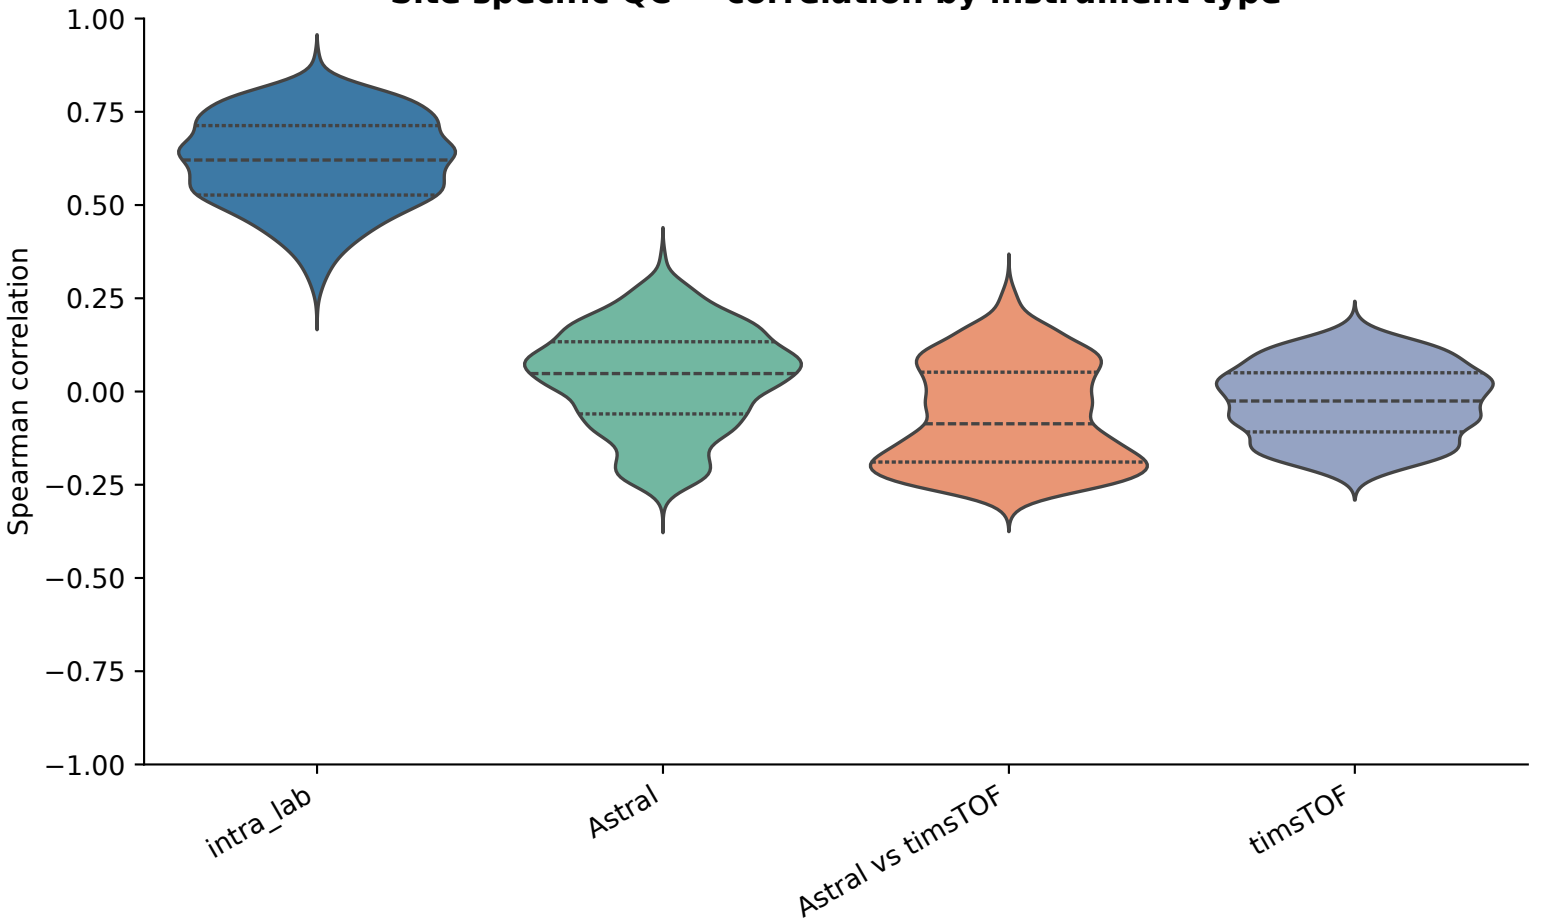
Site specific QC — correlation by instrument type
Spearman correlation
1.00
0.75
0.50
0.25
0.00
−0.25
−0.50
−0.75
−1.00
intra_lab
Astral
Astral vs timsTOF
timsTOF