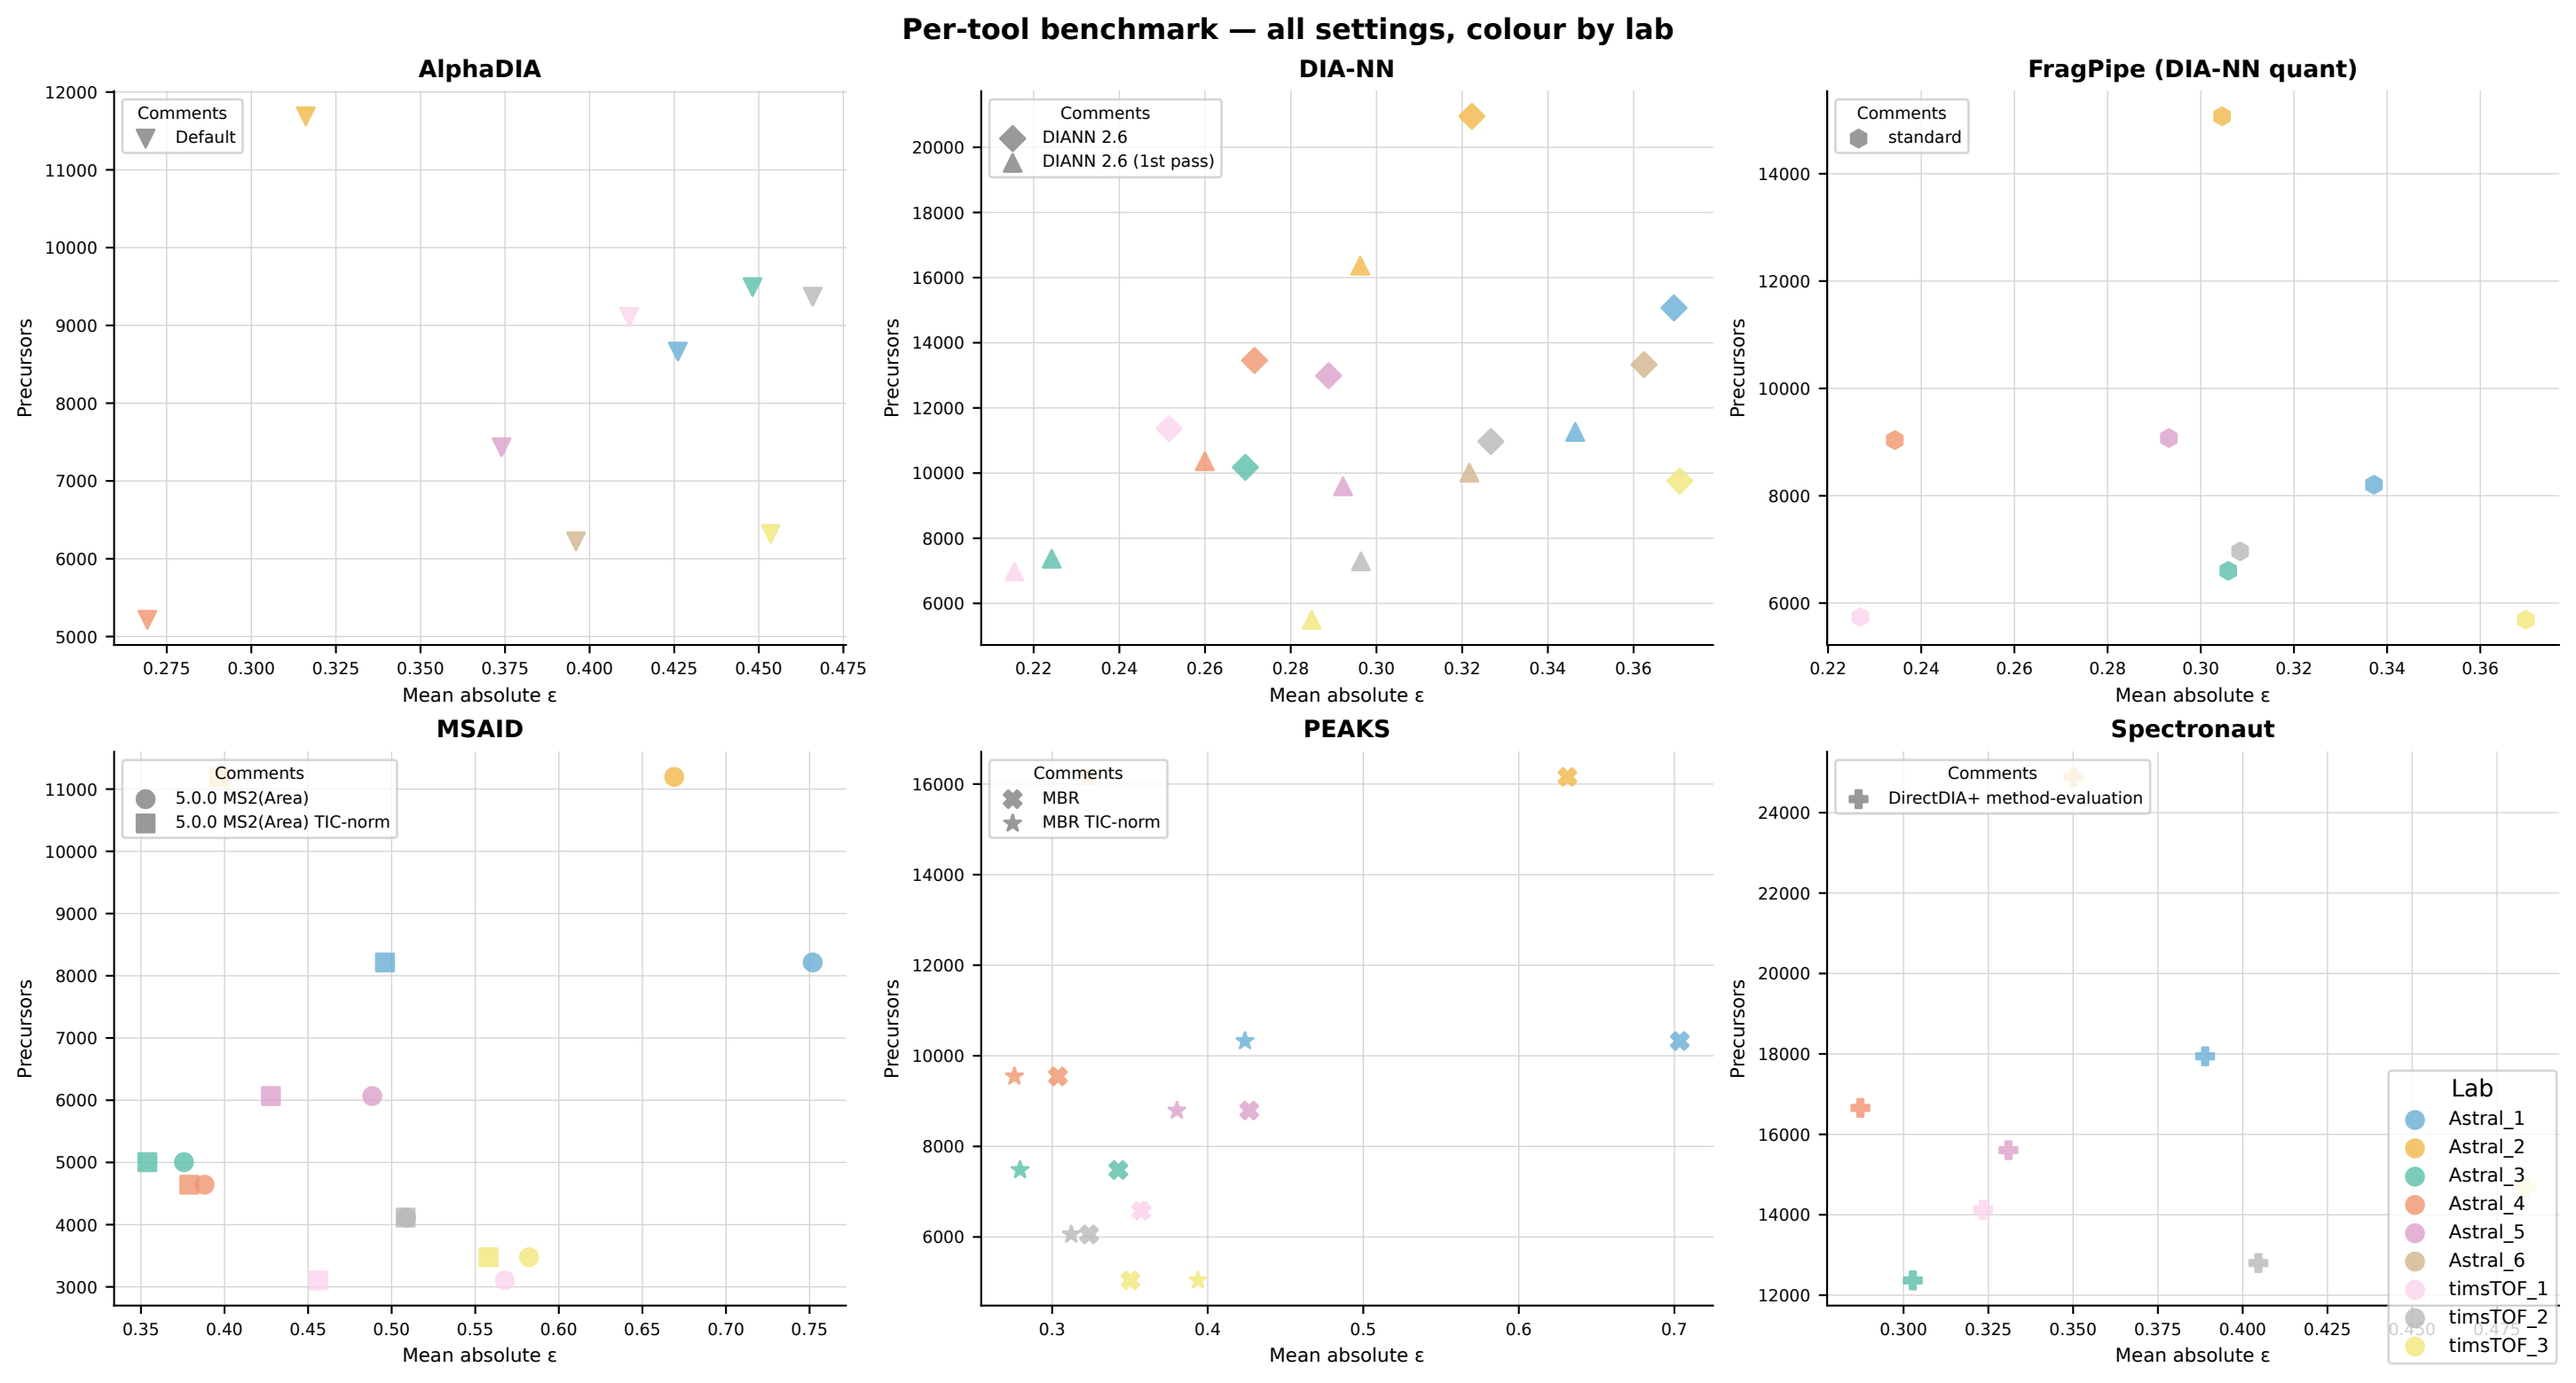
Per-tool benchmark — all settings, colour by lab
AlphaDIA
DIA-NN
FragPipe (DIA-NN quant)
MSAID
PEAKS
Spectronaut
Comments
Default
DIANN 2.6
DIANN 2.6 (1st pass)
standard
5.0.0 MS2(Area)
5.0.0 MS2(Area) TIC-norm
MBR
MBR TIC-norm
DirectDIA+ method-evaluation
Precursors
Mean absolute ε
Lab
Astral_1
Astral_2
Astral_3
Astral_4
Astral_5
Astral_6
timsTOF_1
timsTOF_2
timsTOF_3