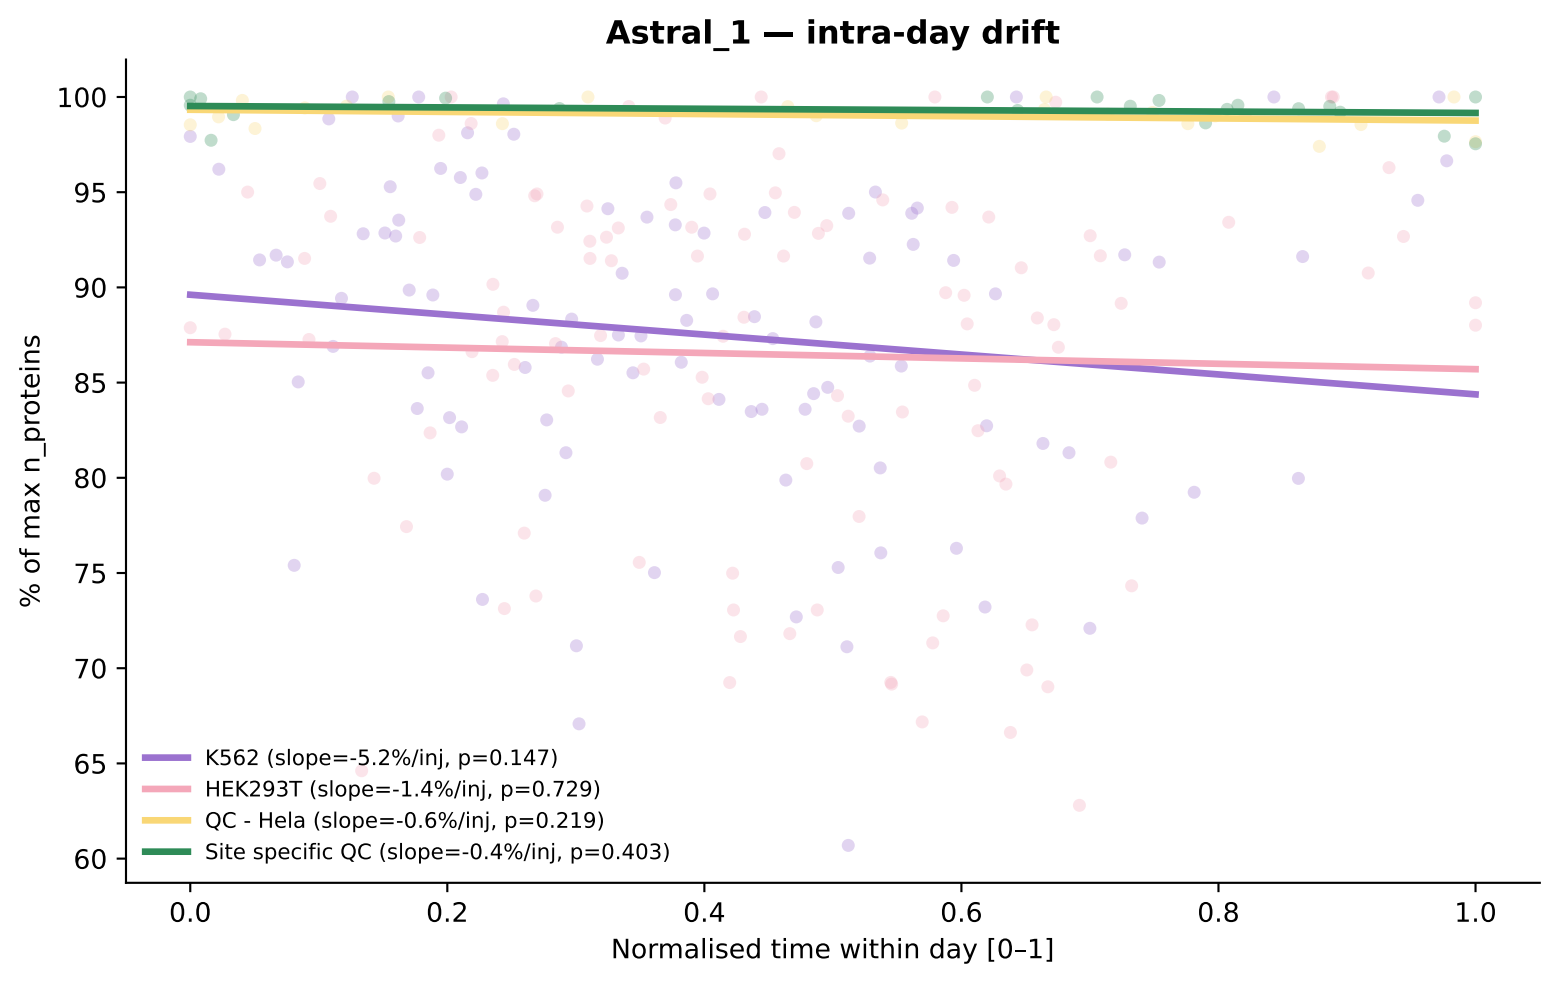
Astral_1 — intra-day drift
% of max n_proteins
Normalised time within day [0–1]
K562 (slope=-5.2%/inj, p=0.147)
HEK293T (slope=-1.4%/inj, p=0.729)
QC - Hela (slope=-0.6%/inj, p=0.219)
Site specific QC (slope=-0.4%/inj, p=0.403)