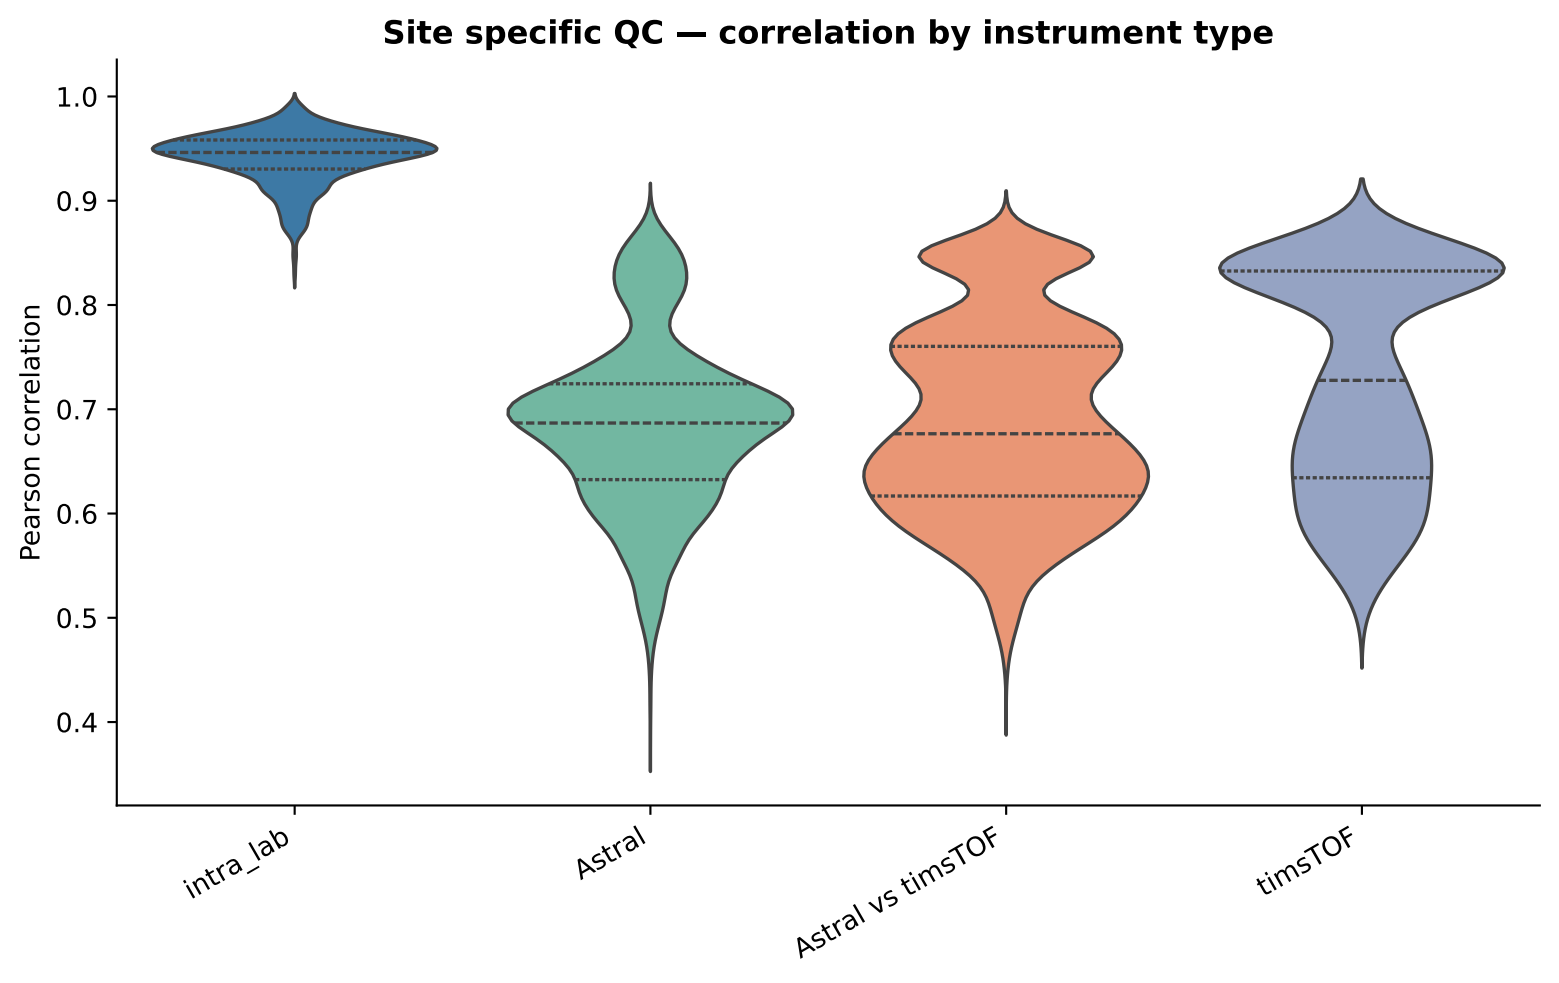
Site specific QC — correlation by instrument type
Pearson correlation
1.0
0.9
0.8
0.7
0.6
0.5
0.4
intra_lab
Astral
Astral vs timsTOF
timsTOF