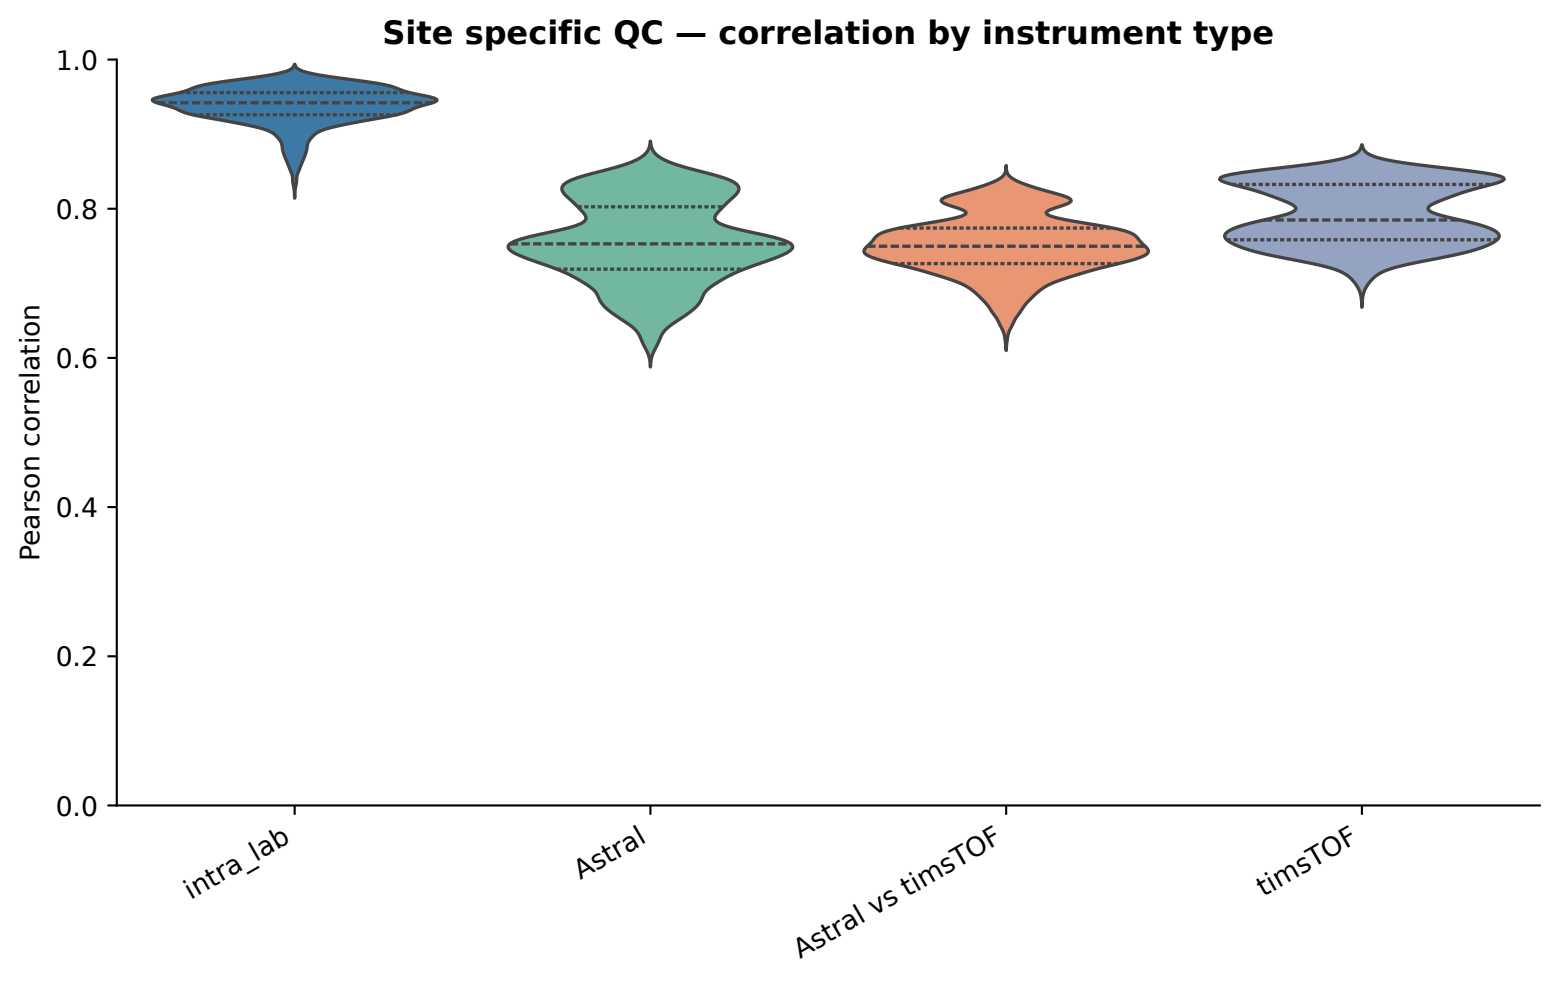
Site specific QC — correlation by instrument type
Pearson correlation
1.0
0.8
0.6
0.4
0.2
0.0
intra_lab
Astral
Astral vs timsTOF
timsTOF