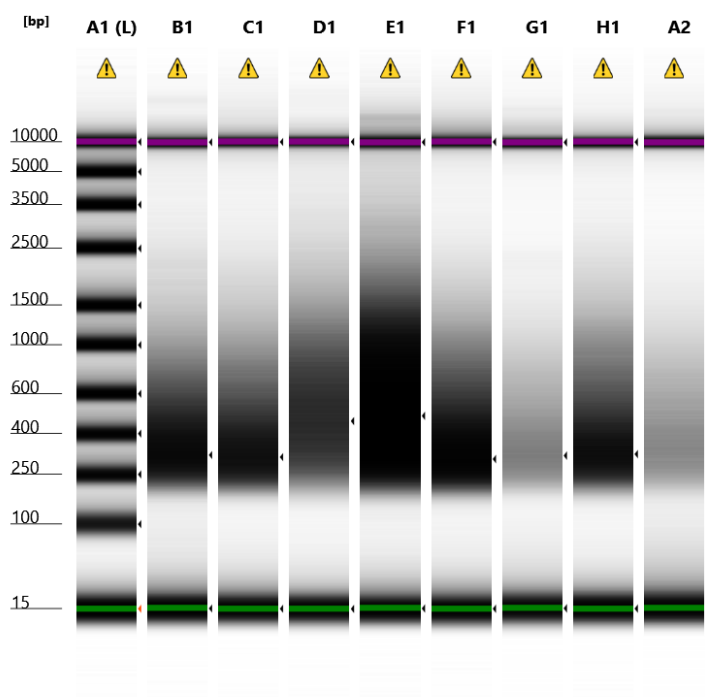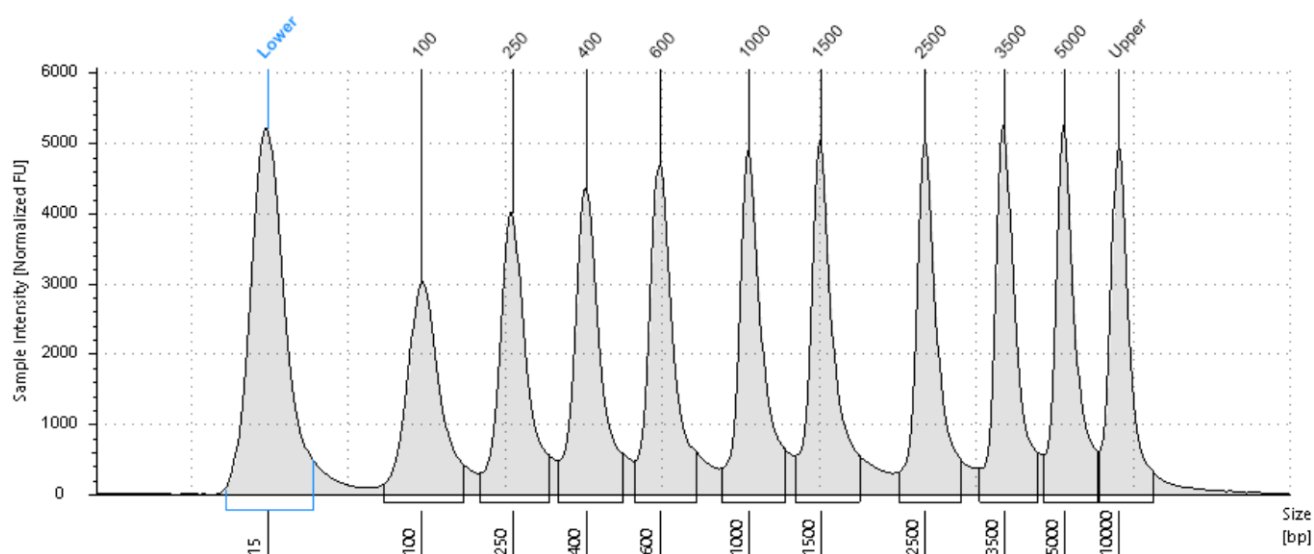## Filename: 2021-04-23 - 10.20.58.D5000

Default image (Contrast 100%)

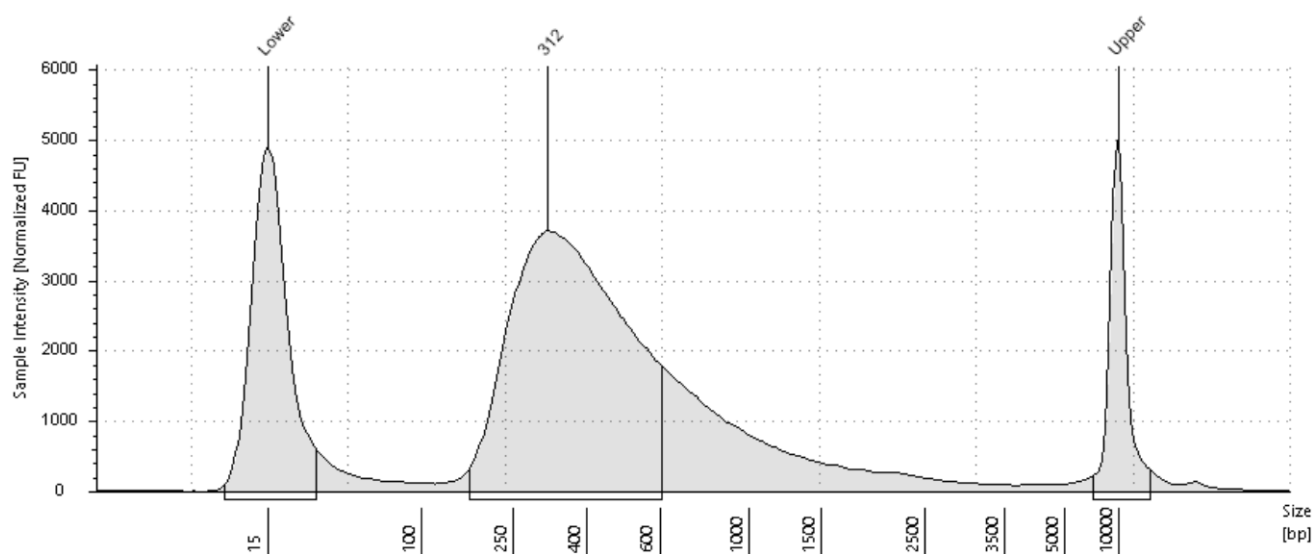## Sample Info

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	43.9	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	20.7	7	⚠	Caution! Expired ScreenTape device
C1	19.4	8	⚠	Caution! Expired ScreenTape device
D1	4.45	9	⚠	Caution! Expired ScreenTape device
E1	34.8	10	⚠	Caution! Expired ScreenTape device
F1	23.4	11	⚠	Caution! Expired ScreenTape device
G1	6.36	12	⚠	Caution! Expired ScreenTape device
H1	19.2	13	⚠	Caution! Expired ScreenTape device
A2	3.61	14	⚠	Caution! Expired ScreenTape device

A1: Ladder

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	43.9	Ladder	⚠️	Caution! Expired ScreenTape device; Ladder

Peak Table

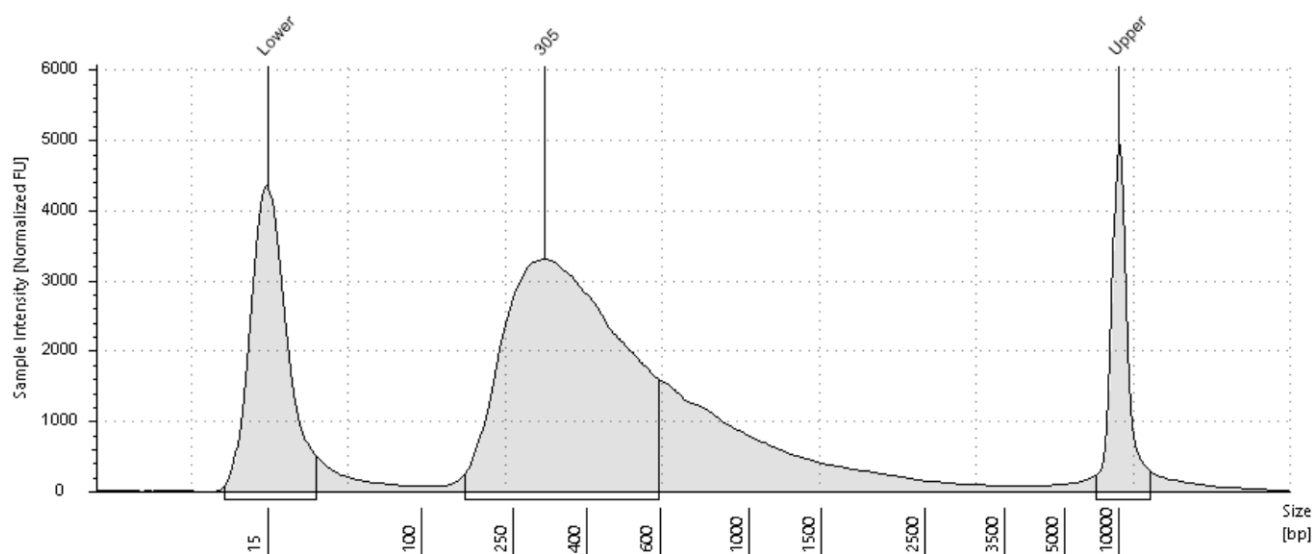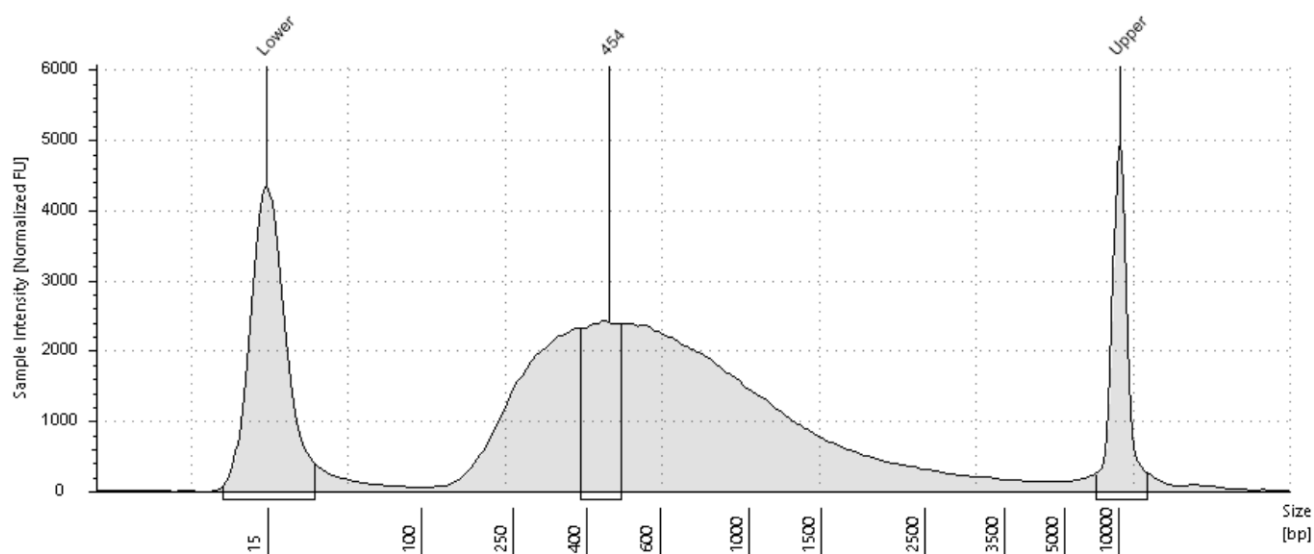| Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.11	-	729	-		Lower Marker
100	4.43	-	68.1	10.08		
250	4.80	-	29.5	10.91		
400	4.95	-	19.1	11.27		
600	5.07	-	13.0	11.54		
1000	5.09	-	7.82	11.57		
1500	5.16	-	5.29	11.74		
2500	4.82	-	2.97	10.97		
3500	4.84	-	2.13	11.01		
5000	4.79	-	1.47	10.90		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 7

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	20.7	7	⚠️	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.10	-	729	-		Lower Marker
312	20.7	-	102	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: 8

Sample Table

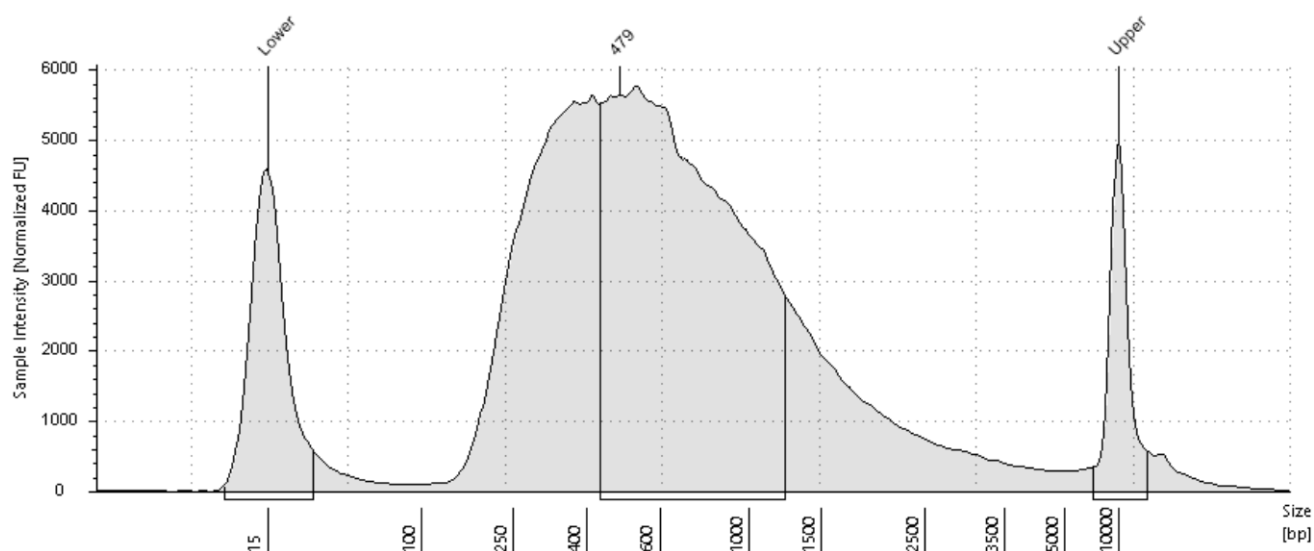| Well	Conc. [ng/µl]	Sample Description	Alert	Observations
C1	19.4	8	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.71	-	688	-		Lower Marker
305	19.4	-	97.6	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

D1: 9

Sample Table

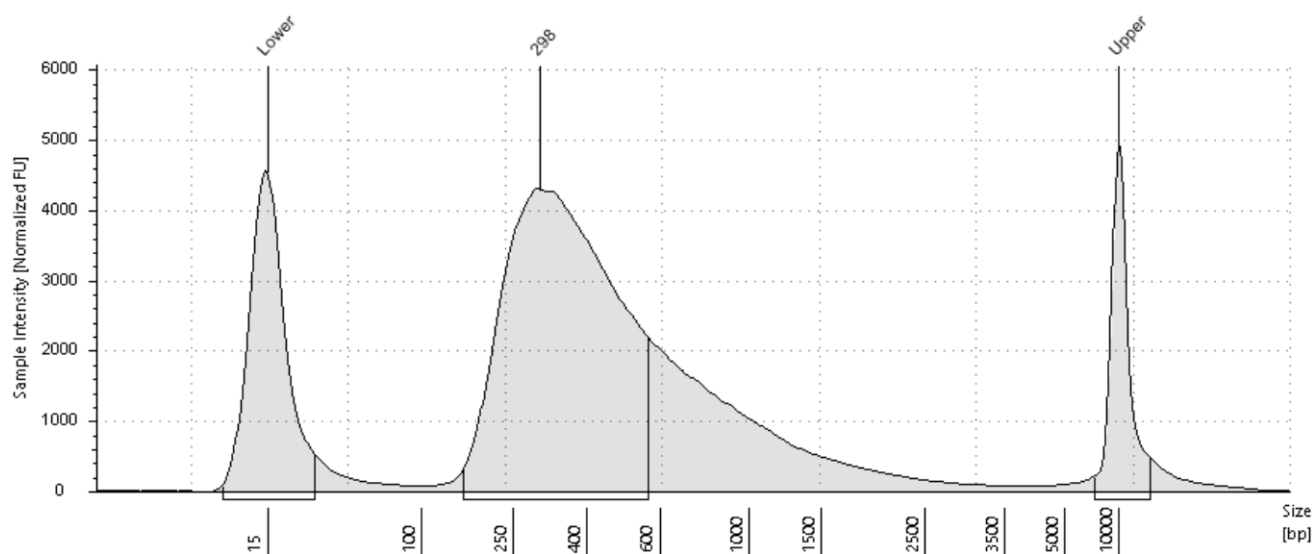| Well	Conc. [ng/µl]	Sample Description	Alert	Observations
D1	4.45	9	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.92	-	709	-		Lower Marker
454	4.45	-	15.1	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

E1: 10

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
E1	34.8	10	⚠	Caution! Expired ScreenTape device

Peak Table

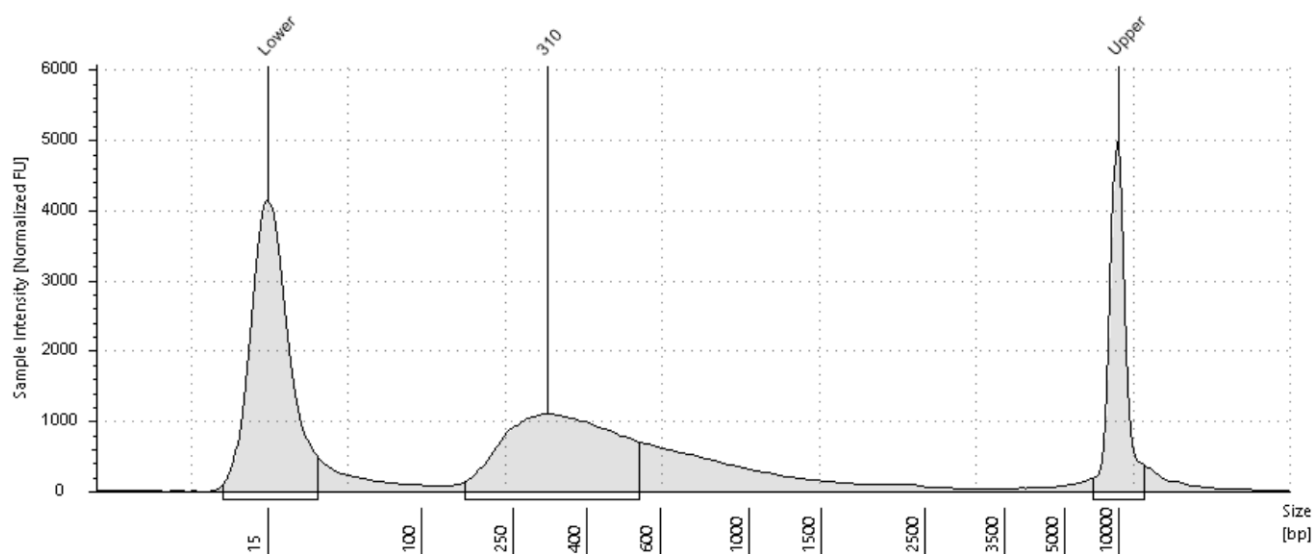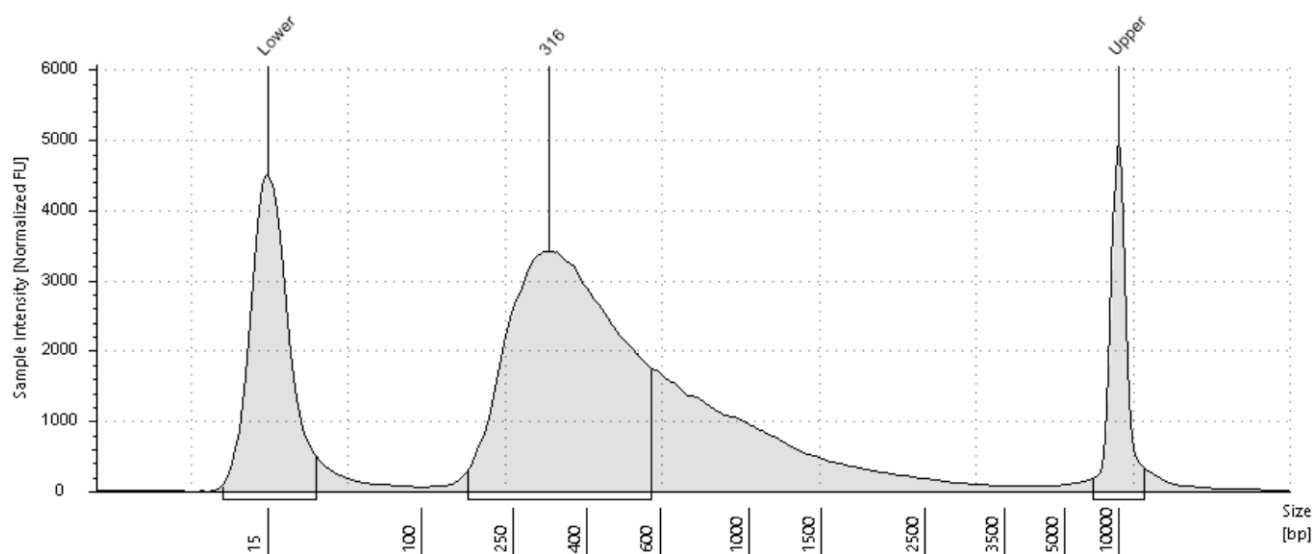| Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.27	-	643	-		Lower Marker
479	34.8	-	112	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

F1: 11

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
F1	23.4	11	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.63	-	680	-		Lower Marker
298	23.4	-	121	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

G1: 12

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
G1	6.36	12	⚠	Caution! Expired ScreenTape device

Peak Table

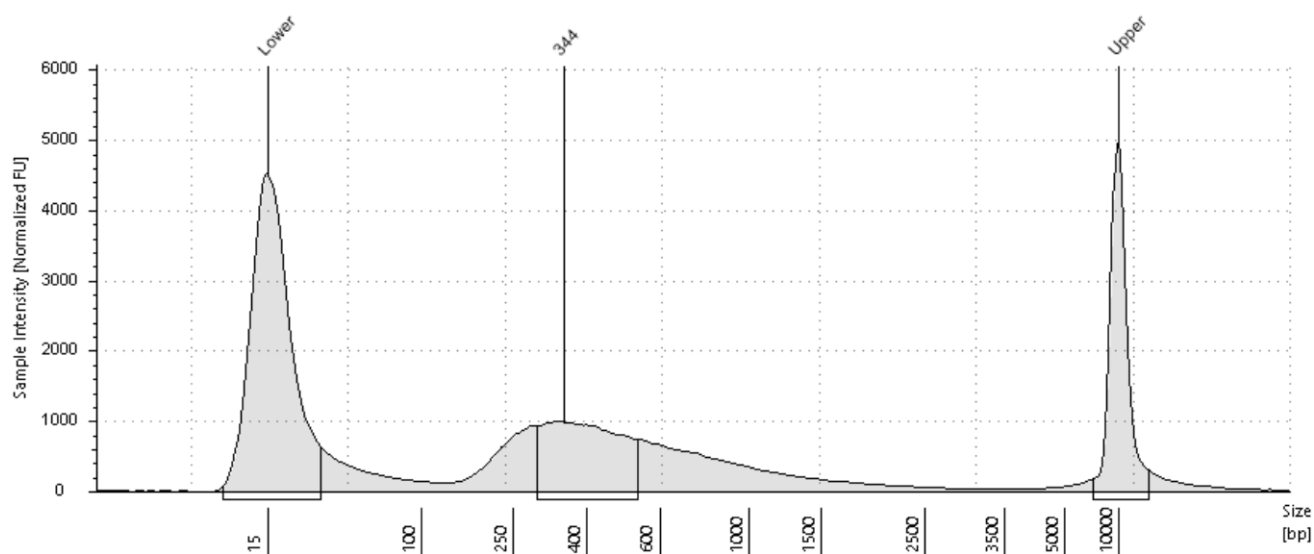| Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.77	-	694	-		Lower Marker
310	6.36	-	31.6	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

H1: 13

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
H1	19.2	13	⚠️	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.40	-	759	-		Lower Marker
316	19.2	-	93.7	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

A2: 14

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A2	3.61	14	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.79	-	696	-		Lower Marker
344	3.61	-	16.1	100.00		
10000	3.25	3.25	0.500	-		Upper Marker