U-W-135B
January 15, 1976
SUPERSEDING
Int. Fed. Spec. U-W-00135A(DSA-DM
March 26, 1970 and
Fed. Spec. U-W-135
July 31, 1947

FEDERAL SPECIFICATION

WAX, BASEPLATE, DENTAL

This specification was approved by the Commissioner, Federal Supply Services, General Services Administration, for use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers dental baseplate wax suitable for forming occlusal rims and setting up artificial teeth.

1.2 Classification. Dental baseplate wax shall be furnished in the following types and classes as specified (see 6.1).

Type I. Medium wax for temperate weather.

Class 1 - Sheets.
Class 2 - Ribbon form.

Type II. Hard wax for hot weather.

Class 1 - Sheets.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

PPP-B-585 - Boxes, Wood, Wirebound.
PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 - Boxes, Shipping, Fiberboard.
PPP-B-676 - Boxes, Setup.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

Federal Standard:

Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specification:

MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

U. S. Department of Health, Education, and Welfare:

Food and Drug Administration.

Federal Food, Drug and Cosmetic Act and regulations promulgated thereunder.

(Application for copies should be addressed to the Division of Public Information, Food and Drug Administration, Washington, DC 20201.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material. Materials used in the formulation of the wax shall be of high quality and suitable in all respects for the purpose intended. The wax shall be free from extraneous materials such as dirt or lint, shall contain no harmful impurities, and shall have no odor or taste other than that characteristic in waxes normally used for this purpose. Content of specific ingredients used in the formulation of the wax (see 3.1.1 and 3.1.2) shall be determined by reference to manufacturer's batch formula records.

3.1.1 Type I, medium wax. Type I, medium wax shall be composed essentially of high quality, synthetic waxes with a maximum of 7.0 percent beeswax, and shall be free from particulate fillers and liquid diluents.

3.1.2 Type II, hard wax. Type II, hard wax shall consist essentially of mineral waxes (such as paraffin or microcrystalline), plant waxes, and beeswax with resins as an additive. A maximum of 1 percent of filler or opacifier is permissible.

3.2 Description. The baseplate wax shall be suitable for forming occlusal rims and for setting up artificial teeth in denture construction. The wax shall be furnished clean and shall be suitable for use in the mouth in trial dentures. The wax shall have a smooth surface appearance. Type I wax shall be a medium wax suitable for use in temperate weather. Type II wax shall be a hard wax suitable for use in hot weather. Class 1 wax shall be furnished in sheet form and Class 2 wax shall be furnished in ribbon form. Wax shall be furnished in the type and class as specified (see 6.1).

3.2.1 Unit of issue. Unless otherwise specified (see 6.1) one box containing a minimum of 5 pounds of wax (type I, class 1) or one box containing a minimum of 1 pound of wax (type I, class 2) or one box containing a minimum of 0.5 pound of wax (type II, class 1), as specified, constitutes one unit of issue.

3.3 Shape and dimensions.

3.3.1 Class 1 wax. The wax shall be provided as individual sheet or scored multiple sheets. Individual sheets shall measure 5-7/8 $\pm$ 1/8 inches (in.) in length, 2-7/8 $\pm$ 1/16 in. in width, and 0.050 $\pm$ 0.005 in. in thickness. Multiple sheets shall measure 8-15/16 $\pm$ 1/8 in. in width, 5-7/8 $\pm$ 1/8 in. in length, and 0.050 $\pm$ 0.005 in. in thickness. Each multiple sheet shall have two scored lines so that when the sheet is broken, three sheets are obtained. Each of the separated sheets shall comply with the dimensions for an individual sheet.

3.3.2 Class 2 ribbon form. The wax shall be furnished in ribbon form in a continuous roll measuring 5-1/2 $\pm$ 1/2 in. in diameter. The roll shall be wound around a sturdy roller and placed in a dispensing box with a side slot to permit ready withdrawal of the desired length of wax. The ribbon of wax shall measure 1-1/2 $\pm$ 1/16 in. in width and 0.050 $\pm$ 0.005 in. in thickness.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

3.4 Weight. The wax shall be furnished in the following minimum weights for the applicable type and class as shown in Table I:

TABLE I. Weight

Type	Class	Minimum weight in pounds
I	1	5.0
I	2	1.0
II	1	0.5

3.5 Color. The color of the baseplate wax shall be pink to simulate appearance of gingival and alveolar tissues. Any color additives used shall be approved and certified by the Food and Drug Administration under the Federal Food, Drug and Cosmetic Act. The baseplate wax shall conform to the standard sample for color (see 3.6, 3.14, 4.4.1 and 6.3).

3.6 Working properties and color. The wax shall have the necessary working properties for proper formation of occlusal rims and trial denture set ups. The wax shall be flexible and shall trim easily without chipping or flaking When gently softened over the flame of a bunsen burner, the wax shall become moldable without crumbling, granulating, flaking, or laminating. When spot warmed with a heated wax spatula, the wax shall soften slightly, but not to a degree that the wax flows from the spatula. When spot heated with a fine flame point, the wax shall flow to produce a smooth glossy surface without loss of its molded form or anatomical detail. The wax shall cool quickly to a firmness which will render it capable of:

a. being carved with a sharp knife without dragging or sticking.
b. retaining porcelain and plastic teeth in proper position.

The working properties of the wax shall be equal to the standard sample when tested as specified in 4.4.1. The sheets (class 1) of the type I wax shall be compatible with the standard sample wax of the ribbon form (class 2) of the type I wax when tested as specified in 4.4.1. The ribbon form (class 2) of the type I wax shall be compatible with the standard sample wax of the sheets (class 1) of the type I wax when tested as specified in 4.4.1.

3.7 Irritation. Unless otherwise specified (see 6.1), prior to delivery, the manufacturer shall furnish a statement directly to the Technical Services Branch, (Code ATTS-2), Directorate of Medical Materiel, Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, stating that the material does not normally irritate oral tissues and does not contain poisonous ingredients in sufficient concentration to be harmful to human beings when used as directed, or in the event of the accidental ingestion of 10g.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

3.8 Physical properties.

3.8.1 Residue and coloring material. The molten wax shall show no color separation or insoluble substance, when tested as specified in 4.4.2.

3.8.2 Flow. The wax shall conform to the flow limits specified in Table II, when tested as specified in 4.4.3.

TABLE II. Flow limits

Temperature ± 0.1°C	Percent flow (type I)		Percent flow (type II)	
	Minimum	Maximum	Minimum	Maximum
21.0	0.0	0.3	0.0	0.2
37.0	0.0	1.6	0.0	1.2
45.0	60.0	85.0	20.0	44.0

3.8.3 Linear shrinkage. The wax shall have a linear shrinkage not exceeding 0.60 percent, when tested as specified in 4.4.4.

3.8.4 Breaking point. At no point on the wax specimen shall there be a complete fracture after 10 seconds, when tested as specified in 4.4.5. A slight craze after 10 seconds will be permitted.

3.9 Adhesion on storage. The adhesion on storage of the wax shall be such that when tested as described in 4.4.6, there shall be no evidence of damage to the wax surfaces that were in contact with each other or with the paper, where separating paper is used, and the wax and paper surfaces shall separate cleanly and readily.

3.10 Lot or control number. Each unit box shall bear the lot or control number and date of manufacture.

3.11 Stability. The baseplate wax shall conform to the requirements of this specification for not less than two years from date of manufacture when stored in a cool place (59° to 86° Fahrenheit (F)). A slight change in the color of the wax will be permitted.

3.12 Delivery schedule. Not more than four months shall have elapsed from date of manufacture of the wax to date of delivery to the Government.

3.13 Workmanship. Workmanship shall be first class throughout. The baseplate wax shall be free from defects which detract from its appearance or may impair its serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

3.14 Standard sample. Unless otherwise specified, as a minimum requirement, the baseplate wax shall be equal to the standard sample for the characteristics of color, working properties and compatibility for which the standard sample is referenced (see 3.5, 3.6, 4.4.1, and 6.3).

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the items.

4.1.3 Certificates of compliance. Certificates of compliance, supplied by the manufacturer of the component or raw material, may be furnished in lieu of actual performance of such testing by the contractor. When certificates of compliance are submitted, the Government reserves the right to check test such items to determine the validity of the certification.

4.1.4 Inspection of materials and components. In accordance with 4.1, the supplier is responsible for insuring that materials and components used were manufactured, tested, and inspected in accordance with the requirements of referenced subsidiary specifications to the extent specified, or, if none, in accordance with this specification. In the event of conflict, this specification shall govern.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered are classified as specified in Tables III, V and VI (see 4.2.1, 4.3 and 4.3.1), and Table IV (see 4.2.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in Table III. Unit of product for examination purposes shall be unit of issue (see 5.1.1). A minimum of 3 sheets from type I, class 1 and type II, class 1 only shall be examined from each unit of product. A minimum length of 12 in. from type I, class 2 only shall be examined from each unit of product.

TABLE III. Inspection and Acceptable Quality Levels (AQL's)

Type defect	Inspection level	AQL (Percent defective)
Major	S-2	1.5
Minor	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with Table IV, except that the acceptance number shall be zero for all sample sizes. Sufficient number of sheets (type I, class 1 and type II, class 1) and sufficient quantity of ribbon form wax (type I, class 2) shall be drawn at random from each of two boxes per lot or control number.

TABLE IV. Tests

Characteristic	Rqmt.	Test Procedure	Number of Determinations
Working properties and color	3.6	4.4.1	3 1/
Residue and coloring material	3.8.1	4.4.2	2 1/
Flow	3.8.2	4.4.3	5 2/
Linear shrinkage	3.8.3	4.4.4	2 2/
Breaking point	3.8.4	4.4.5	3 1/
Adhesion on storage	3.9	4.4.6	3/

1/ A lot shall be rejected if any determination fails the test requirement.

2/ Result shall be the average of the individual values obtained from the number of specimens taken from each lot.

3/ Two complete boxes of wax, packaged as specified in 5.1.2.1.1 or 5.1.2.1.2 shall be tested.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

4.3 Examination. Wax shall be examined for defects, including, but not limited to, those listed in Table V.

TABLE V. Classification of Defects

Categories	Defects
Major:	
101	Type and class (shape) not as specified.
102	Color not as specified.
103	Surface of wax not smooth.
104	Odor or taste not as specified.
105	Wax not furnished in shape specified.
106	Wax not clean, presence of foreign matter.
Minor:	
201	Dimensions not as specified for specific type and class.
202	Weight not as specified for specific type and class.

4.3.1 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table VI. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with AQL of 4.0 expressed in terms of percent defective.

TABLE VI. Examination of preparation for delivery

Examine	Defect
Contents	Not as specified.
Container	Not as specified.
Marking	Omitted; incorrect; illegible; improper size, location, sequence or method of application.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

TABLE VI. Examination of preparation for delivery (continued)

Examine	Defect
Material	Component missing or damaged.
Workmanship	Bulging or distoration of containers.

4.3.1.1 Examination of closure, waterproofing and banding of container. When the shipping container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the box specification.

4.4 Tests.

4.4.1 Working properties and color. Practical tests shall be performed to determine compliance with the requirements of 3.5 and 3.6 by comparing the working qualities and color of the test wax with the standard sample wax (see 3.14). The wax shall be tested at 75 ± 5° F for type I wax and 90 ± 5° F for type II wax. To test for compatibility, an equal amount of the test wax and standard sample wax of the applicable type I class 1 and 2 waxes shall be softened to moldable consistency and combined to form an occlusal rim.

4.4.2 Residue and coloring material. An upper base plate of plastic shall be constructed using acceptable dental procedures. Plastic teeth shall be waxed on one side and porcelain teeth shall be waxed on the other side of the wax model denture. The wax model denture shall be constructed using the wax (type I or II) being tested. The wax model denture shall be flasked in the usual manner using dental plaster or stone or both. The flask shall be allowed to set on the bench for at least two hours after the final set of the plaster. It shall then be placed into a water bath at 50° ± 5° C for ten minutes, at which time the flask halves shall be separated and the bulk of the base plate shall be stripped out. The flask shall then be flushed with three applications of a boiling solution of synthetic household detergent (1 tablespoon to 1 pint of water) and rinsed with clean boiling water. The wax shall not leave a visually detectable residue on the porcelain or plastic teeth nor shall the coloring material separate from the wax or impregnate the plaster.

4.4.3 Flow test.

4.4.3.1 Preparation of specimens. A sufficient number of sheets or rolls of wax shall be broken into pieces and placed in an iron crucible of 50 milliliter (ml) capacity. The crucible shall be placed 130 millimeters (mm) below a 250-watt infrared lamp bulb. The stirred wax shall be heated to a temperature of 75° ± 5 Centigrade (C) (check with a thermometer) until melted throughout and then shall be poured into a mold (Figure 1). The mold shall be a flat,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

stainless steel metal plate 6.0 mm thick, containing four holes 10.0 mm in diameter. The mold shall be preheated to a temperature of 55° ± 5° C and placed on a smooth glass slab (150 mm long, 75 mm wide, 20 mm thick) which shall have been preheated to the same temperature. After the mold has been overfilled with material, a smooth, flat, tinfoil-covered glass plate, preheated to 55° ± 5° C, shall be placed on top of the mold. A load of 90 newtons (N) shall be applied to the top of the tin-foil glass plate for 10 minutes. Then the mold shall be placed in water at a temperature of 10° C for 10 minutes. The upper tin-foiled plate shall then be removed and the excess material shall be trimmed away. This can be accomplished by using a metal scraper with the top surface of the mold as a guide. The mold may then be removed from the glass slab by gently tapping the side of the mold. The specimens shall be removed from the mold by chilling in water for 10 minutes at 10 C, and shall be stored at room temperature, 23° ± 2° C, for 24 hours before testing.

4.4.3.2 Method of test. The original length of the specimen shall be determined using a metric micrometer caliper. Four measurements shall be made around the circumference and one measurement shall be made on the center of the specimen. The measurements shall be recorded to the nearest 0.005 mm. The specimen and flow testing instrument (Figure 2) shall be placed in a water bath and held at the testing temperature for 20 minutes prior to testing. The flow testing instrument as illustrated consists of the following: A, a weight; B, a nonconducting shaft; and C, a brass platen. The total weight in air of these three components is 19.6 N. The weight A shall be separated a minimum of 75 mm from the brass platen on the shaft. This shaft shall be of hard rubber or of a similar poor thermal conductor to avoid loss in heat due to conduction. The diameter of the brass platen which touches the specimen shall be no less than 50 mm. The thickness of the brass platen shall not exceed 6.5 mm. The temperature in the bath shall be controlled to within ± 0.1°C of the required temperature. A thin sheet of waterproof cellophane shall be placed between the instrument and each end of the specimen. The bottom of the specimen shall be 51 mm below the surface of the water in the bath. A constant axial load of 19.6 N shall then be applied to the specimen for 10 minutes, after which the specimen shall be removed and cooled in air to room temperature. The cellophane shall be stripped off, and the final length shall be determined as is the original length. The flow, as evidenced by the change in length, shall be reported as percentage of the original length. The value for flow at any temperature shall be the average value for five specimens from each lot (control number) and shall be reported to the nearest 0.1 percent.

4.4.4 Linear shrinkage. Specimens for determination of linear shrinkage shall be prepared in a like manner to the flow test specimens. Linear shrinkage shall be determined on a specimen 200 to 300 mm in length and with equipment sufficiently accurate to insure correct results within plus or minus 0.05 percent. The wax shall be chilled from 40.0 ± 0.1° C to 25.0 ± 0.1° C and the linear shrinkage determined. Two specimens from each lot (control number) shall be tested, and the average shall be reported. The percent of linear shrinkage shall be the difference in specimen length at the two temperatures, divided by the length at 40° C, multiplied by 100.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

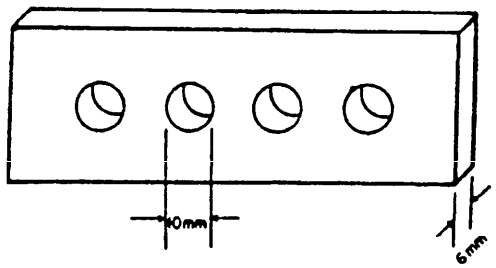


FIGURE 1 —Mold for forming flow specimens.

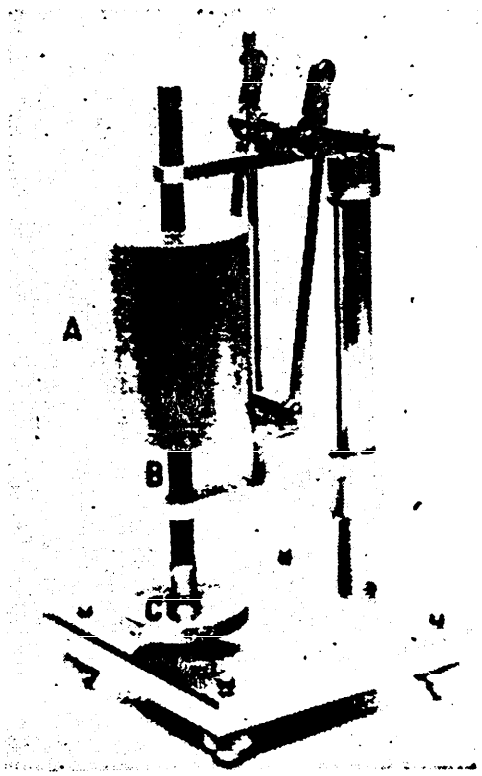


FIGURE 2 —Flow testing instrument. A; weight B: nonconducting shaft. C: platen.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

4.4.5 Breaking point. At a temperature of 21° ± 1° C for type I wax and 27° ± 1°C for type II wax, the baseplate wax shall be bent at a uniform rate for ten seconds until it is bent double, with the two halves of the specimen in contact throughout their entire length. The bend shall be perpendicular to the longer dimension of the specimen. Three specimens shall be tested.

4.4.6 Adhesion on storage. Three specimens of wax and a specimen of separating paper, where such is used, having dimensions of 5 cm wide and 7.5 cm long shall be prepared. The specimen shall then be placed between two platens 5 cm wide, 6 cm long, and 0.5 cm thick in such a manner that 1.5 cm of each wax specimen projects from one end of the platens, and the separating paper, where used, is between two of the wax specimens. The assembled specimens shall then be placed in an oven maintained at a temperature of 40 ± 1.0 C° for Types I and II on a flat rigid surface and a weight of 13.2 N including the weight of the top plate shall be applied. At the end of 24 hours the specimens shall be removed and allowed to cool to room temperature. At the end of two hours the specimens shall be separated by opening from the overlapping ends, and the surfaces in contact with other specimens shall be examined for evidence of damage.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Unit package.

5.1.1.1.1 Type I, class 1 and Type II, class 1. One half pound of Type II, class 1 or five pounds of type I, class 1 shall be packaged in a box constructed in accordance with PPP-B-676. Sheets shall be interleaved with suitable paper to prevent binding or blocking when stocked one upon another. The paper used for interleaving shall be of such compatibility that the wax will not be altered in any way. Closure of the box shall be as specified in the appendix of the box specification.

5.1.1.1.2 Type I, class 2. One pound of ribbon wax shall be packaged as specified in 3.3.2.

5.1.1.2 Intermediate package. Twelve unit packages containing type I, class 2 wax shall be packaged in a snug fitting box constructed in accordance with PPP-B-636, type CF, class domestic. Closure of the box shall conform to method I as specified in the appendix of the box specification. Intermediate package shall not be required for type I, class 1 and type II, class 1 wax.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.1).

5.2.1 Level A. Ten unit packages containing type 1, class 1 wax or ninety-six unit packages containing type II, class 1 wax or four intermediate packages containing type 1, class 2 wax shall be packaged in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.2 Level B. Ten unit packages containing type 1, class 1 wax or ninety six unit packages containing type II, class 1 wax or four intermediate packages containing type II, class 1 wax shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, constructed so as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123. The shipping container shall be marked with the legend:

"STORE AT CONTROLLED ROOM TEMPERATURE (59° - 86° F)."

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable box is fabricated of water-resistant material. Lot (control) number, contract or purchase order number, name of contractor, date of manufacture (in lieu of date packed) and the following legend shall be shown:

"STORE AT CONTROLLED ROOM TEMPERATURE (59° - 86° F)."

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. The lot (control) number shall be shown. The date of manufacture shall be shown in lieu of the date packed. Marking shall include the following legend:

"STORE AT CONTROLLED ROOM TEMPERATURE (59° - 86° F)."

6. NOTES

6.1 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents:

(a) Title, number, and date of this specification.
(b) Type and class required (see 1.2 and 3.2).
(c) If statement of irritation is to be furnished to another Government activity (see 3.7).
(d) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(e) If unit of issue other than that specified (see 3.2.1).

6.2 Conversion factors.

25.4mm (2.54cm) = 1 inch
(°C x 1.8) + 32° = °F
453.59g = 1 pound
9.807N = 1 kilogram force

6.3 Standard sample. For access to standard sample, address the procuring activity issuing the invitation for bids or request for proposal (see 3.5, 3.6, 3.14 and 4.4.1).

MILITARY CUSTODIANS:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activities:

COM - NBS
GSA - FSS
HEW - FDA, HSM
VA - DMS

Preparing activity:

DSA - DM

Project No. 6520-1379

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. **Price 40 cents each.**

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute, or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
U-W-135B - WAX, BASEPLATE, DENTAL

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

☆ GPO: 1974— 603-680/6126 2-1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:20Z
Check the source to verify that this is the current version before use.