GG-H-00575c(DSA-DM)
24 April 1967
Interim Revision of
Fed. Spec. GG-H-575b
14 May 1957

INTERIM FEDERAL SPECIFICATION

HOLDER, NAPKIN, DENTAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-H-575b.

1. SCOPE

1.1 Scope. This specification covers a napkin holder suitable for holding linen or disposable patient towels in proper position during dental operative procedures.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-123 Marking for Domestic Shipment (Civilian Agencies).

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

(Copies of Military specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Materials. The napkin holder chain shall be made of brass, chrome over nickel plated. The clasp jaws shall be made of brass, chrome plated, or carbon steel, chrome over nickel over copper plated. The clasp pin and spring shall be made of steel spring wire, suitably plated to protect against corrosion. The clasp sleeves shall be made of a cast phenolic material.

3.2 Style, design and dimensions. The dental napkin holder, covered by this specification, shall be provided with an alligator-jaw type, spring closure at each end of a flexible beaded chain. Each clasp shall be provided with a crimping section at the base for accommodation of the chain, and shall have a protective sleeve cover at the juncture of the clasp and ball chain. The napkin holder shall be in conformance with Figure 1 for style, design and dimensions.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3.2.1 Chain. The chain shall be extremely flexible and shall be used to connect the two clasps. The chain shall be of the ball-chain type and shall consist of a series of balls linked together by "dumbbell type" links.

3.2.2 Clasps. The clasps shall be constructed to mesh properly when in closed position, and shall hold the napkin securely while in use.

3.2.2.1 Sleeves. The sleeves shall be designed to adequately protect the juncture of the chain and clasp. The sleeves shall provide a means of gripping the clasp portion of the napkin holder, and shall serve as a housing for the crimped section of the clasp and chain.

3.2.2.2 Clasp spring and pin. The spring and pin in each clasp shall serve the joint function of tieing the two clasp jaws together and maintaining the pressure necessary to hold the jaws in a closed position. The spring shall be wound to give a spring tension of 10 ± 3 pounds, when tested as specified in 4.4.1.

3.3 Corrosion resistance. Each napkin holder shall pass the boil test when tested as specified in 4.4.2.

3.4 Identification marking. Each napkin holder shall be permanently and legibly marked with the name or registered trademark of the manufacturer.

3.5 Workmanship. Workmanship shall be first class in every respect. The removal of a slight amount of plated material, while crimping the clasp around the chain, shall be acceptable.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The Inspection Levels and Acceptable Quality Levels (AQL's) shall be as indicated in Table I.

Table I. Acceptable Quality Levels

Type Defect	Inspection Level	AQL (Percent Defective)
Major A	II	1.0
Major B	S-1	2.5
Minor	II	4.0

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics. Acceptance number shall be zero for all sample sizes.

Table II. Tests

Characteristic	Requirement	Test procedure	Unit of product	Inspection level
Spring Tension	3.2.2.2	4.4.1	1-napkin holder	S-2
Boil Test	3.3	4.4.2	1-napkin holder	S-2

4.3 Examination. Dental napkin holders shall be examined for defects including, but not limited to, those listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical:	None defined.
Major A:	
101	Alligator jaws do not mesh properly.
102	Napkin holder components not assembled properly.
103	Napkin holder has large cracks in sleeves, burrs, sharp edges, or slivers.
104	Style and design of napkin holder not as specified.
Major B:	
121	Number of clasp teeth not as specified.
122	Dimensions of napkin holder not as specified in Figure 1.
Minor:	
201	Plated components show signs of peeling or flaking.
202	Identification marking missing or illegible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

4.4 Tests.

4.4.1 Spring tension test. A spring type, platform scale, having a minimum range of 10 pounds and graduations of 2 ounces or less, shall be used to test the spring tension of the alligator jaw clasp. The clasp shall be placed in the center of the scale platform. The clasp shall be held firmly in the position shown on the right hand side of Figure 1. Pressure shall be slowly applied to the clasp finger rest until the upper jaw is parallel to the lower jaw. The scale pointer registration shall then be recorded. The test shall be repeated three times and an average of the results shall represent the spring tension of the clasp.

4.4.2 Boil test. Before testing,the napkin holder shall be scrubbed with soap and water, rinsed thoroughly in distilled water, and dried. After cleaning, the holder shall be boiled in distilled water in a glass beaker for 30 minutes and allowed to remain submerged for an additional 24 hours. A slight corrosion in pin, spring or in crimped area of clasp shall be acceptable.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One holder, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable. Closure shall be adequate to prevent spilling of contents under normal handling. As an alternate, each unit shall be packaged in a transparent plastic envelope of suitable size and design, closure of which shall be adequate to prevent accidental opening.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

5.1.3.2 Intermediate package. Intermediate package shall be a carton of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic and method I closure shall be utilized.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, constructed so as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Civilian agencies. Marking for shipment in accordance with FED-STD-123.

5.3.2 Military agencies.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown. The required information for each unit package may be printed on a label inserted within the plastic package, if used in such a manner as to permit ready identification.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not cover all types, classes, grades or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

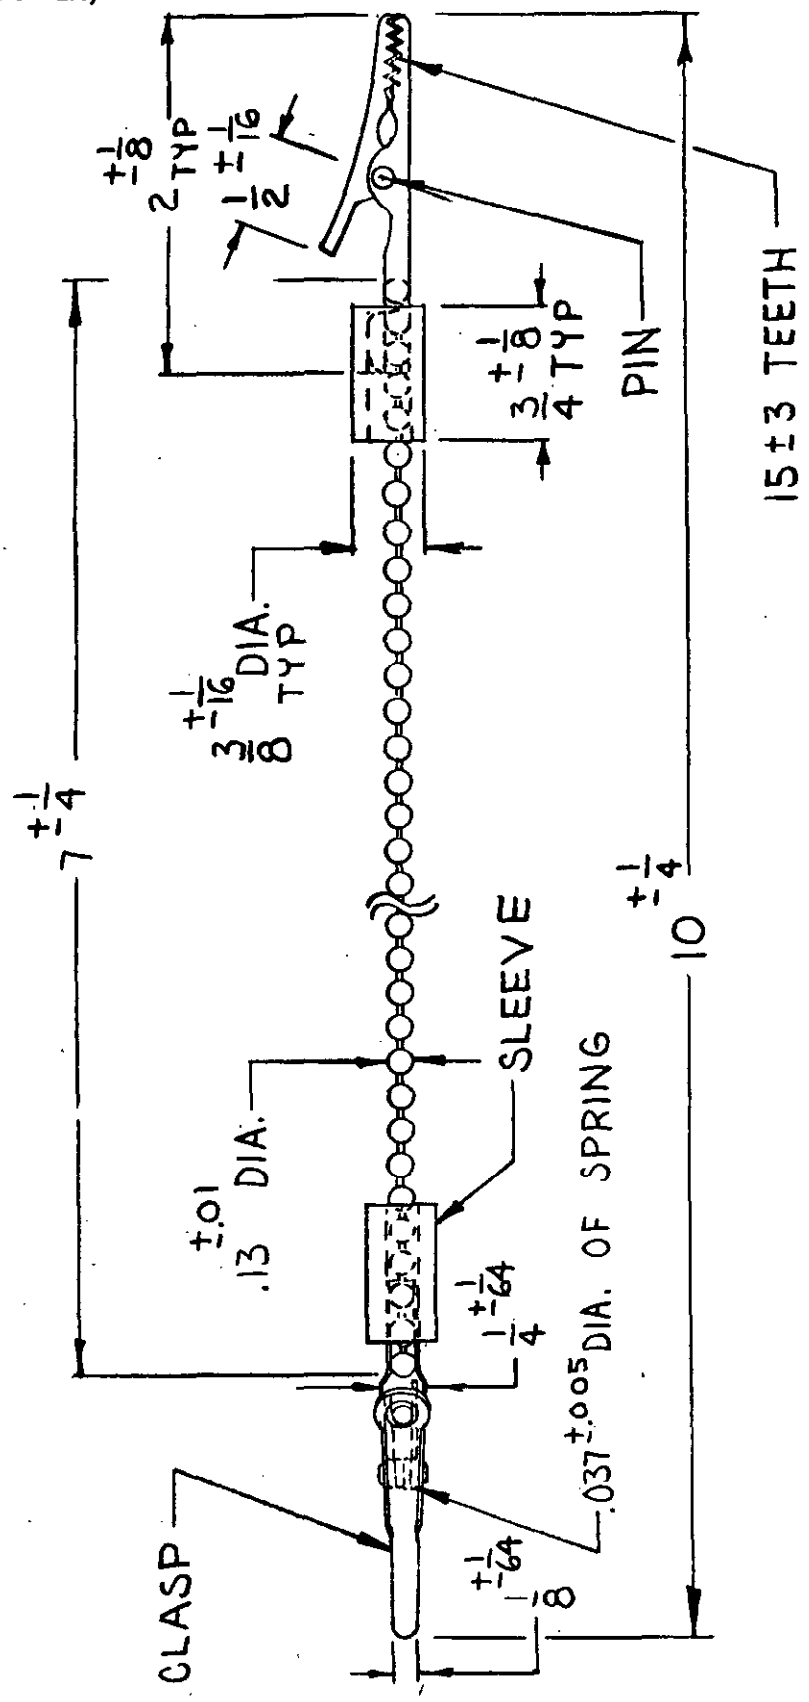


FIGURE 1. HOLDER, NAPKIN, DENTAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
AUG 66

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

GG-H-00575c(DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.