GG-H-00590a (DSA DM)
22 July 1966
Interim Revision of
Fed. Spec. GG-H-590
14 January 1959

INTERIM FEDERAL SPECIFICATION

HOLDER, RADIOGRAPHIC FILM CASSETTE

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-H-590, dated 14 January 1959.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers a vertical type cassette holder designed for wall mounting and suitable for holding standard radiographic film cassettes, and a standard radiographic stationary grid.

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND OTHER PUBLICATIONS

2.1 Specifications, standards, and drawings. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

L-P-509	Plastic Sheet, Rod and Tube, Laminated, Thermosetting.
QQ-A-200/3	Aluminum Alloy, Bar, Rod, Shapes and Tube, Extruded, 2024.
QQ-A-591	Aluminum Alloy Special Shaped Sections.
QQ-A-601	Aluminum-Alloy Sand Castings.
QQ-S-698	Steel, Sheet and Strip, Low Carbon
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

FSC 6525

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

Military

MIL-F-1148	Fiber, Vulcanized, Electrical and Mechanical Grades.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

Federal

FED-STD-151	Metals, Test Methods.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C., 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and standards from established distribution points in their agencies.)

(Copies of specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Preproduction sample. Unless otherwise specified (see 6.1), prior to the start of production of the contract quantity, one preproduction sample of the cassette holder shall be assembled, completely finished, and tested by the contractor. The sample shall be submitted, together with the contractor's inspection and test reports, to the contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the contracting officer, or his authorized representative, prior to the manufacture and assembly of the remaining quantity to be manufactured. Further production of the item by the contractor, prior to this approval, shall be at the contractor's risk. Accepted preproduction sample shall become the property of the procuring activity and shall be included in the quantity called for in the contract or order. In the event that the preproduction sample is not approved, the contractor shall submit a new sample for approval, or modify the existent sample so as to remove the deficiencies cited.

3.2 Material. Satisfactory high grade materials shall be used throughout. Materials shall be suitable for the purpose and of sufficient strength to maintain operational alignment for life of the equipment.

3.2.1 Steel, sheet, plate, and strip stock. Steel sheet, plate, and strip stock shall conform to the requirements of QQ-S-698 when tested as specified in 4.4.1.

3.2.2 Aluminum. Cast aluminum shall conform to the requirements of QQ-A-591 or QQ-A-601 and aluminum tubing shall conform to the requirements of QQ-A-200/3, Temper T81, when tested as specified in 4.4.1.

3.2.3 Bushings. Bushings may be metallic or nonmetallic. Metallic bushings shall be brass; nonmetallic bushings shall be fiber conforming to grade BH, form S, of MIL-F-1148, nylon or laminated thermosetting plastic conforming to type II, grade C, of L-P-509.

3.3 Construction. The wall mounted cassette holder shall be constructed as shown in figure 1. The holder shall consist of the following components:

Mounting base----------3.3.1
Carriage track----------3.3.2
Cassette carriage----------3.3.3
Chinrest----------3.3.4
Height indicator----------3.3.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3.3.1 Mounting base. The mounting base shall consist of one or more rigid sheet metal plates. Suitably placed holes for mounting the unit to the wall, and the accessories for mounting the unit, shall be provided.


3.3.2 Carriage track. There shall be suitable tracks or channels to hold the cassette carriage. The carriage tracks shall be chrome-plated steel, corrosion-resisting steel solid bars, tubular steel (corrosion-resistant or chrome-plated), or aluminum tubing, and shall be smooth, parallel and of a sufficient length to permit a range of motion of at least 15 inches with a 14- by 17-inch cassette mounted on the cassette carriage with its long axis vertical. The minimum wall thickness of all tubing shall be 0.049 inch.

3.3.3 Cassette carriage assembly. The cassette carriage shall be reinforced with steel and shall move freely and smoothly in a vertical direction. There shall be a locking device to permit locking the cassette carriage at any point in its vertical travel. The cassette carriage shall be adjustable to hold and lock in place any standard type cassette, with the cassette in either the horizontal or vertical position. The cassette carriage shall be marked to facilitate centering of cassettes. The front of the cassette carriage shall be open so that the cassette is always in view as an aid to centering. In addition, there shall be grooves, tracks, or a guide rail to support the 14- by 17-inch grid close to the cassette, when any size cassette from 5 by 7 inches to 14 by 17 inches is being used in either horizontal or vertical position. An adjustable cassette adapter, as specified in 3.3.3.1, shall be supplied so that any standard size cassette may be used with a standard 14- by 17-inch grid. The bushings, riding the carriage tracks, when fabricated of a nonmetallic material shall be encased between two sheets of steel and the assembly securely and permanently fastened to the carriage, or as an alternate, the bushing may be mounted directly on the carriage by means of rivets. The nonmetallic bushings shall be approximately 3/32 inch thick and shall make contact with the carriage tracks in at least eight points (four on each side). The brass bushings may be full length for each section for a total of four bushings. As an alternate method of construction, the upper and lower carriages may be fabricated as aluminum castings, drilled to accommodate the vertical guides. When this method of construction is used, bushings shall not be required.

3.3.3.1 Adjustable cassette adapter. The adjustable cassette adapter shall be fabricated of aluminum or sheet steel. The adapter shall have a clamping device 1-7/8 inches long for holding the cassette, and a locking device, such as knurled thumbscrew (setscrew) to lock the cassette in place.

3.3.4 Chinrest. Chinrest shall be of cast aluminum or other suitable material. The chinrest shall be highly polished and shall have no sharp corners or edges. The chinrest shall be permanently fastened to the top edge of the cassette carriage. The chinrest shall be shaped to the contour of the chin so as to facilitate positioning of the patient in chest radiography.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

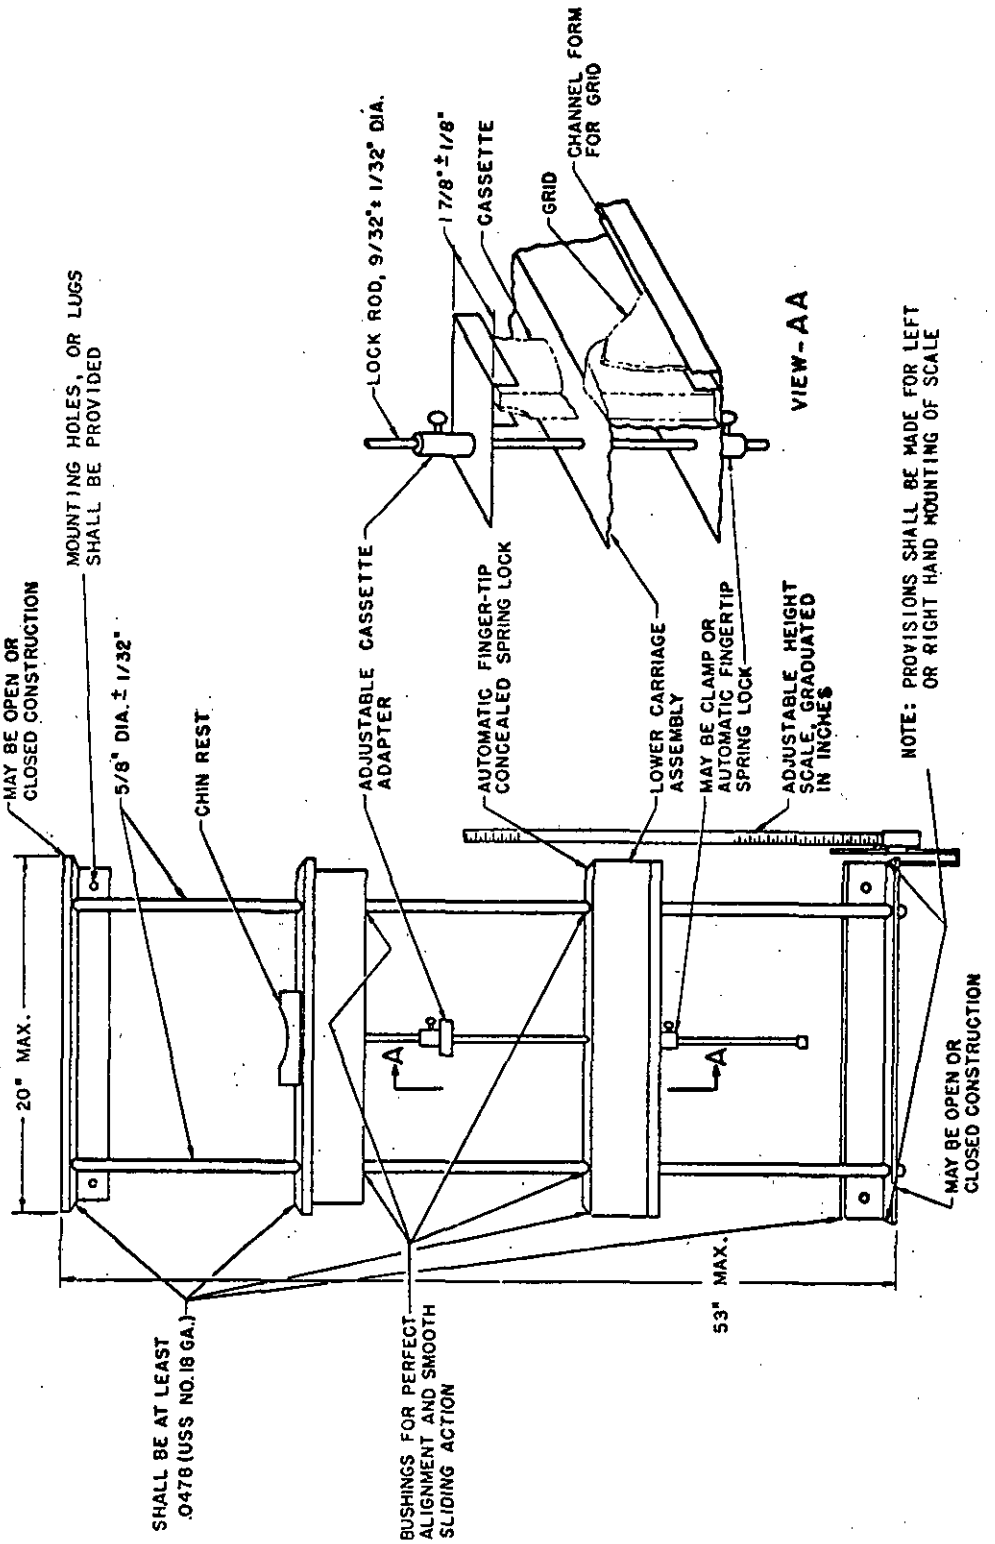

NOTE: FIGURE SHOWN IS TYPICAL OF STYLE AND DESIGN ONLY.

FIGURE 1.

10 March 1965

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

3.3.5 Height indicator. A height indicator fabricated of sheet steel shall be furnished. The height indicator shall be graduated in inches and shall be constructed so as to become an integral part of the cassette holder. The height indicator shall be numbered to help in aligning the cassette carriage with the X-ray tube. The height scale shall be adjustable to correspond to the tabletop or cassette to focal spot scale on any X-ray tubestand. Height indicator shall be interchangeable for right-or left-side mounting.

3.4 Finish. The wall mounted cassette holder shall be degreased, primed, and finished with smooth enamel in the manufacturer's standard color. Trimming shall be chrome or other suitable corrosion-resistant material. The finish shall not fade, crack or peel under normal conditions of use.

3.5 Interchangeability. All individual parts or assemblies of parts of any complete unit supplied on a contract shall be interchangeable with corresponding parts of assembly of parts of all other units supplied on that contract.

3.6 Identification marking. Each wall mounted cassette holder shall have a metal nameplate permanently marked, or shall be stamped with the following information, and located to permit reading without difficulty:

Manufacturer's name or registered trademark.
Manufacturer's type and model number.
Contract or purchase order number.
Federal stock number.
Letters U.S.

Marking secured by adhesives shall not be used.

3.7 Service data. The contractor shall furnish, with each unit, two copies of service data containing complete instructions for installation, operation, maintenance, and a list of component parts. All information contained in the manual shall be suitably indexed to permit ready reference to the required information so that the replacement parts can be ordered by the manufacturer's part number, and without confusion as to the item identification. Identical or interchangeable replacement parts shall be identified by a single part number only. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the contracting officer two preliminary copies of his proposed service data for review and comment (see 6.1). The preliminary service data shall be submitted sufficiently early to permit adequate review (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of required revisions and corrections in the final service

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T11:51Z
Check the source to verify that this is the currentversion before use.

data without delaying delivery under the contract or purchase order. In addition, the contractor shall mail 15 copies of the approved service data to the contracting officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of contract, and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request.

3.8 Workmanship. Workmanship shall be first class throughout. The wall mounted cassette holders shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

	Inspection level	AQL (defects per hundred units)
For visual examination Major defects	II	1.0
Total (major and minor combined) defects	II	4.0
For dimensional examination	S-1	6.5

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

4.2.2 Raw materials. Four ounces of each lot of each metal used in the construction of the holder shall be selected for chemical analysis (see 4.4.1).

4.3 Examination. The holder shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Inspection shall be conducted in accordance with the following classifications of defects:

Categories and defects*

Major

101 Holder not complete with all specified component parts.
102 Cassette carriage fails to slide smoothly and freely over the entire length of its travel.
103 Locks on either cassette carriage or adjustable cassette adapter fail to fix or release at any set position.
104 Adjustable cassette adapter fails to slide smoothly and freely over the length of its travel.
105 Channels in upper and lower horizontal members of carriage assembly, including cassette adapter, not properly located and aligned to accommodate cassette and grid.
106 Component parts not free of cracks and burs or sharpness at edges.
107 Plating not free of blistered, excessively scratched or unplated areas.
108 Cassette carriage adjustment not within range required to hold any standard type cassette in vertical or horizontal position.
109 Height indicator scale not present or not graduated as specified.
110 Height indicator scale not adapted for right- or left-side mounting.

Minor

201 Cassette carriage not marked to facilitate centering cassettes.
202 Finish not smooth, adherent and free of chipped, cracked, blistered, or bare areas.
203 Identification marking not present and complete or not permanent and legible.
204 Service data, in duplicate, not included with each unit.

*Inspection is not restricted to the classified defects listed above.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The holder shall be inspected for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted in accordance with the applicable specifications to determine compliance with this specification.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Fed. Test Method Std. No. 151.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One holder, as specified, constitutes one unit of issue, one each.

5.1.2 Level A.

5.1.2.1 Unit package. Each unit shall be packaged in a carton of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall conform to applicable paragraph of appendix thereto.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Each unit package shall be overpacked in an exterior container designed for type 1 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class Weather-resistant.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix of PPP-B-636. In addition, waterproofing shall be as specified in 30.4 of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the current version before use.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. No overpacking of unit package for level B protection shall be required.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Where preproduction sample shall be sent (see 3.1).
(c) Where service data shall be sent (see 3.7).
(d) Selection of applicable levels of packing (see 5.1 and 5.2.)

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.