FEDERAL SPECIFICATION

INCUBATOR BACTERIOLOGICAL, LARGE

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

This specification forms a part of the latest issue of GG-I-488/GEN.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers the specific requirements for an air circulating gravity convection type incubator with water reservoir.

1.2 Classification. The bacteriological incubator covered by this specification shall be of one type.

2. APPLICABLE DOCUMENTS

The latest issue of GG-I-488/GEN and the documents referenced therein.

3. REQUIREMENTS

3.1 Material. The inner and outer walls, legs, shelves and shelf brackets shall be fabricated of corrosion-resisting steel that conforms to FED-STD-66, AISI 304. The inner walls shall be 0.0239 in. thick (No. 24 Manufacturers Standard Gage) and the outer walls shall be 0.0359 in. thick (No. 20 Manufacturers Standard Gage). The gages shall be considered a minimum and commercial tolerances shall apply.

3.2 Design. The incubator shall be an air circulating gravity convection type, with a water reservoir located below the chamber floor. The incubator shall have four rigid doors: two glass inner doors and two corrosion resisting steel outer doors. The doors shall be so designed to make a tight fit with the cabinet when closed. The incubator shall have suitable openings for adequate and proper ventilation. The incubator shall have an opening at the top to accept the thermometer specified in 3.3.2 of GG-I-488/GEN. The incubator shall be equipped with a minimum of three removable shelves. A water funnel and a drain cock for filling and draining the reservoir shall be located in a compartment on the side of the incubator.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3.3 Dimensions. The cabinet of the incubator shall have minimum inside dimensions of 25 inches high by 37 inches wide by 19 inches deep. The overall outside dimensions shall be approximately 40 inches high by 49 inches wide by 27 inches deep.

3.4 Construction.

3.4.1 Cabinet. The cabinet shall be of the single chamber type and shall have an inner and outer wall on all sides, back, top and bottom. The walls shall be so designed or suitably reinforced that no "oil canning effect" is present. The walls shall be adequately insulated, as specified in 3.3.4 of GG-I-488/GEN, to maintain the temperature range and tolerance specified herein.

3.4.2 Doors.

3.4.2.1 Outer doors. The two corrosion-resisting outer doors shall be of rigid construction, fully insulated and provided with suitable gaskets, or otherwise constructed to insure an air tight fit with the incubator cabinet.

3.4.2.2 Inner doors. The two inner doors shall be constructed of glass having a minimum thickness of 3/16 inch. The glass shall be mounted in a corrosion-resisting steel frame so constructed that the glass is easily removable. The inner doors shall make a tight fit with the cabinet. The inner doors shall have a suitable latch handle having a minimum lever arm of 2 inches. The latch shall be suitably designed and attached to the door to prevent self-opening.

3.4.3 Shelves. The shelves shall be fabricated of rigid wire mesh, perforated metal or expanded metal.

3.4.4 Legs. The incubator shall have four legs suitably designed and constructed to support the weight of the incubator during normal use in the laboratory.

3.5 Electrical components.

3.5.1 Power switch. The incubator shall be provided with a heavy duty power switch for energizing and de-energizing the heater elements.

3.5.2 Pilot light. The incubator shall be provided with a pilot light, with a red lens, visible from the front of the incubator, to indicate when the unit is energized.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

3.6 Power consumption. The rated power consumption shall be 1200 watts.

3.7 Temperature range. The incubator shall be capable of operation at 30°C to 60°C with an accuracy of ± 1/2°C when tested as specified in 4.4.2 of GG-I-488/GEN.

3.8 Workmanship. The workmanship shall conform to GG-I-488/GEN.

4. QUALITY ASSURANCE PROVISIONS

The quality assurance provisions shall conform to GG-I-488/GEN.

5. PREPARATION FOR DELIVERY

Packaging, packing and marking requirements shall be as specified in GG-I-488/GEN.

6. NOTES

6.1 Intended use. This incubator is intended for use in medical laboratories for the incubation of micro-organisms.

6.2 This specification is intended to cover the following item:

National stock number	Item identification
6640-00-428-8120	Incubator, Bacteriological, Large

6.3 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents:

a. Title, number, and date of this specification.
b. National stock number (NSN).
c. Selection of applicable levels of packaging and packing specified in GG-I-488/GEN.

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA-DM

Civil Agency Coordinating Activities:
VA-DMS
HEW-NIH
GSA-FSS

Project No. 6640-0985

Orders for this publication are to be placed with General Services Administration, acting as agent for the Superintendent of Documents. See section 2 of this specification to obtain copies of documents referenced herein. Price 30 cents each.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
GG-I-488/3 INCUBATOR BACTERIOLOGICAL, LARGE

NAME OF ORGANIZATION AND ADDRESS	CONTRACT NUMBER
	MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*


4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

GPO 1974 — 603 680 6126 2 1

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:51Z
Check the source to verify that this is the current version before use.

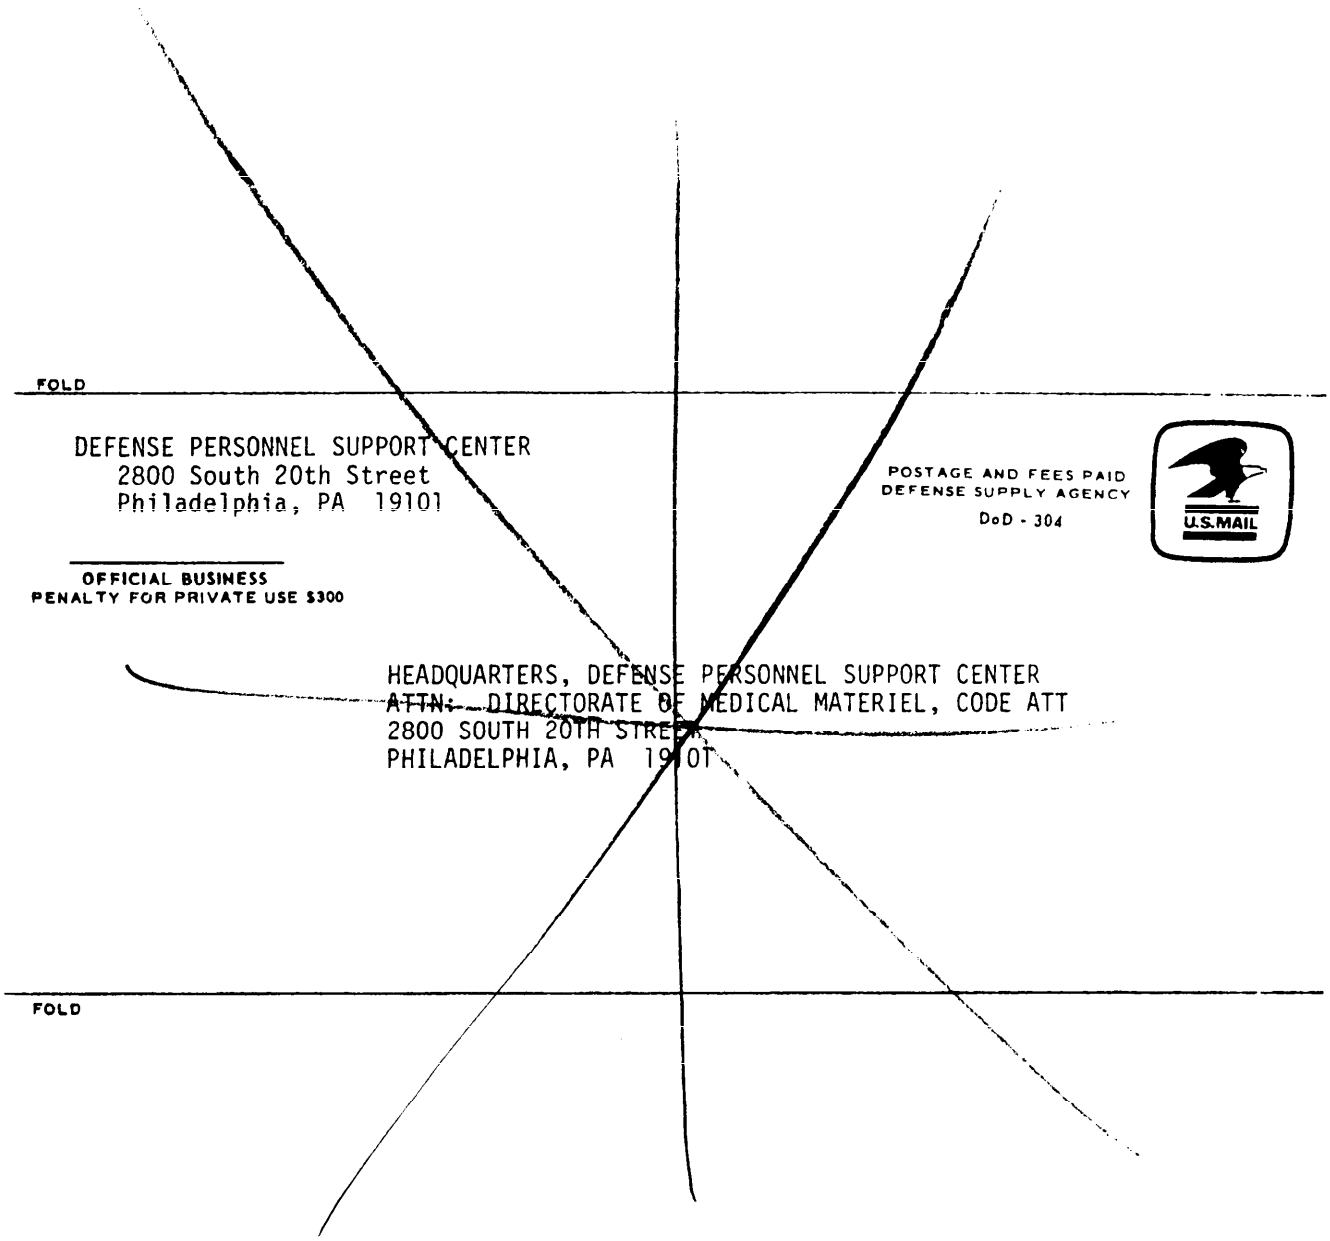

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.