FEDERAL SPECIFICATION

SOUNDS, URETHRAL (CURVED, LEFORT)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers curved urethral sounds capable of union with urethral filiform catheters and suitable for use in urethral dilation.

1.2 Classification.

1.2.1 *Grade, type, and size.*—Urethral sounds shall be of one grade and type, and of the following sizes, as specified in the invitation for bids:

Size 1—12 Fr.
Size 2—14 Fr.
Size 3—16 Fr.
Size 4—18 Fr.
Size 5—20 Fr.

2. APPLICABLE SPECIFICATIONS

2.1 The following Federal Specifications, of the issues in effect on date of invitation for bids, form a part of this specification:

GG–F–340—Filiforms, Urethral, Woven (Braided).
GG–I–526—Instruments, Dental and Surgical: General Specifications.

(Copies of Federal Specifications and the Index of Federal Specifications and Standards may be obtained upon application, accompanied by check, money order, cash, or Government Printing Office coupons, to the General Services Administration, Business Service Center, Region 3, Seventh and D Streets SW., Washington 25, D. C. This office will also honor deposit account numbers issued by the Government Printing Office. Prices may be obtained from the Index of Federal Specifications and Standards or from the GSA Regional Offices. Single copies of this specification and other product specifications required for bidding purposes are available without charge at the GSA Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.)

271928—54—No. 224

2.2 Specifications and standards applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 Material.—Material shall conform to Federal Specification GG–I–526, for class 2, composition G (c).

3.2 Construction.—Urethral sounds shall be LeFort design. Construction shall be of one piece or two piece, and shall conform to illustration as shown in figure 1. Sound shall be so constructed that when fitted with a urethral filiform conforming to Federal Specification GG–F–340, the latter shall be capable of butting against the end of the sound. Sound shall be free from burrs and sharp edges. The standard threads and taper to the threaded joint of the sound shall be identical to the specification of the filiform or vice versa. Threads on end of sound shall be cleanly cut.

3.3 Finish.—Finish shall be in accordance with Federal Specification GG–I–526 for mirror finish.


3.4 Identification marking.—The handle of the sound, toward the concave side of the curve, shall be legibly and permanently marked with the size (in French scale), and the name or trade-mark of the manufacturer.


3.5 Workmanship.—Workmanship shall be first class throughout. Sounds shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.—Unless otherwise specified, at least 2 sounds of each size shall be taken at random from each lot of 100 or fraction thereof delivered.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

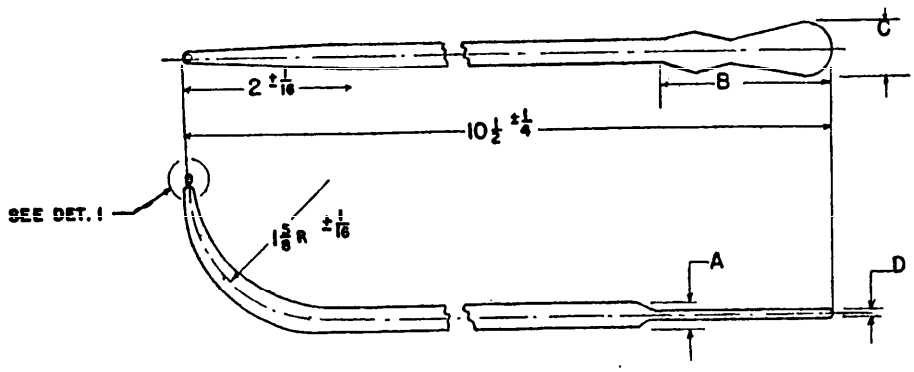

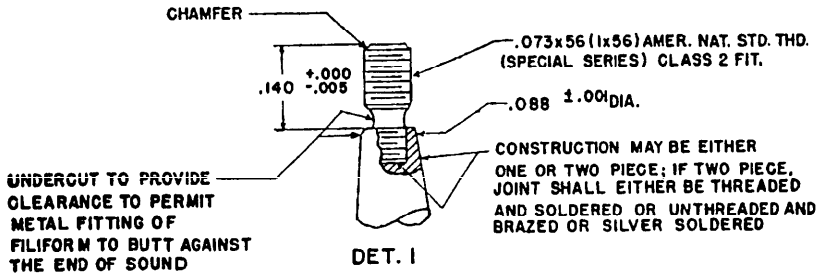

SOUND, URETHRAL, (CURVED LEFORT)

Size	Stock No.	Nomenclature	"A" (French scale)	"B" (inches)	"C" (inches)	"D" (inches)
1	6515–367–9100 (3–679–100)	Sound, urethral, curved, LeFort, 12 fr....	12	1¾	½	3/64
2	6515–367–9120 (3–679–120).	Sound, urethral, curved, LeFort, 14 fr....	14	1¾	½	1/16
3	6515–367–9140 (3–679–140).	Sound, urethral, curved, LeFort, 16 fr....	16	1¾	½	5/64
4	6515–367–9160 (3–679–160).	Sound, urethral, curved, LeFort, 18 fr....	18	1¾	9/16	3/32
5	6515–367–9180 (3–679–180).	Sound, urethral, curved, LeFort, 20 fr....	20	2	9/16	7/64
Tolerances permissible →			±0.1mm	±1/16	±1/16	±0.008

Note.—The French scale is equal to 3 times the size in millimeters.

FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:51Z
Check the source to verify that this is the currentversion before use.

4.2 **Inspection.**—Samples shall be inspected for construction, finish, identification marking, workmanship, packaging, packing, and marking.

4.3 **Tests.**

4.3.1. *Material.*—The material used in the construction of the sounds shall be tested as described in Federal Specification GG-I-526.

5. PREPARATION FOR DELIVERY.

5.1 **Packaging.**—Unless otherwise specified, sounds shall be packaged in accordance with accepted commercial practice.

5.2 **Packing.**—The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate, and to afford maximum protection from normal hazards of transportation.

5.3 **Marking.**

5.3.1 *Packages.*—Unless otherwise specified, packages shall be marked with the name and size of the commodity, the quantity contained therein, and the name of the manufacturer and contractor.

5.3.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked with the name and size of the commodity as defined by the contract or order under which the shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 **Ordering data.**— Purchasers should specify size required, and should exercise any desired options offered herein. (See 1.2, 4.1, 5.1, 5.3, and 6.2.)

6.2 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.3 This specification covers the following items appearing in the Armed Services Medical Stock List:

6515-367-9100—Sound, Urethral, Curved, LeFort, 12 Fr. (3-679-100)

6515-367-9120—Sound, Urethral, Curved, LeFort, 14 Fr. (3-679-120)

6515-367-9140—Sound, Urethral, Curved, LeFort, 16 Fr. (3-679-140)

6515-367-9160—Sound, Urethral, Curved, LeFort, 18 Fr. (3-679-160)

6515-367-9180—Sound, Urethral, Curved, LeFort, 20 Fr. (3-679-180)

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the type, etc., normally procured for Federal Government requirements.

6.5 **Transportation description.**— Transportation description applicable to these items is:

Surgical instruments, not otherwise indexed by name.

Carload weight 10,000 pounds, subject to Rule 34, Uniform Freight Classification.

Truckload weight 10,000 pounds.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specification of the issue in effect on date of invitation for bids, and special requirements, forms a part of this specification for purchases made under this specification by the respective departments.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specification.*

Military Specification:

MIL-P-12902—Packaging of Surgical, Dental and Veterinary Instruments, Diagnostic Equipment, and Related Items.

(Copies of specifications, standards, and drawings required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer).

7.2.2 *Packaging.*

7.2.2.1 *Unit of issue.*—One (1) sound, as specified, constitutes one unit of issue.

7.2.2.2 *Level of protection.*—The required level of protection (Level II, Domestic), (Level III, Overseas), for packaging, packing, and marking shall be as specified in the procurement document for the required number of units of issue.

7.2.3 *Packaging, packing, and marking.*—Packaging, packing, and marking for the specific level of protection shall be in accordance with the requirements of Military Specification MIL-P-12902 for the applicable procedure code number as indicated in table A.

7.2.3.1 *Packaging and packing quantities.*—The number of units of issue to be contained in each unit or intermediate package and shipping container shall be as indicated in table A.

TABLE A

Level of protection	Procedure code No.	Unit pack	Intermediate pack	Shipping container
II Domestic	20	1	6	216
III Overseas	30			

ARMY INTEREST: M
NAVY INTEREST: Md

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:51Z
Check the source to verify that this is the current version before use.