INCH-POUND

A-A-54895
16 July 1993

COMMERCIAL ITEM DESCRIPTION

SOUND CHAMBER AND CUFF, BLOOD PRESSURE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-37123A, which is cancelled.

This Commercial Item Description covers requirements for two sizes of sound chambers unit with blood pressure cuff and bag assembly suitable for indirect blood pressure measurement during surgical procedures.

Salient characteristics:

Scope The blood pressure sound chambers covered by this document shall be of the following sizes:

Size	Sound Chamber
I	Adult
II	Medium Adult

Requirements. The blood pressure sound chamber and cuff unit shall essentially consist of a sound chamber, a cuff and a compression bag.

The blood pressure sound chamber shall be fabricated from a soft neoprene rubber or other suitable material. The sound chamber unit shall consist of a contoured sound chamber with permanently attached metal nipple and attached vinyl sound tube of about 22 inches in length. The nipple shall be made of stainless steel or aluminum. The free end of the sound tube shall be fitted with a male Luer taper suitable for connection to a pair of aural tubes. The male Luer taper shall be in accordance with ISO 594. The top of the sound chamber shall have a strip of hook type fastening strip cemented to it. A complementary strip of pile fastener shall be attached to the sphygmomanometer cuff so that the sound chamber will remain in position during use.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

The sound chamber for each size as specified shall be in accordance with Figures 1a and 1b.

The cuff shall be of one size of appropriate dimensions suitable for use with both adult and medium adult blood pressure sound chambers. The cuff shall include an inflatable compression bag. The cuff shall be held in position around the patient's arm by means of hook and pile tapes appropriately situated and sewn on to the cuff.

The compression bag shall be of seamless construction and shall have an inlet and outlet tube each of which shall be 8 ±1 inches in length. The outlet tube shall be sealed with a removable plug.

The cuff and compression bag shall be legibly and permanently marked with the contractor's name or registered trademark.

Performance. The compression bag shall be capable of withstanding an internal pressure of 12 psig for one minute without leakage.

The cuff and compression bag when steam autoclaved at 29 to 31 psig and 250° ±2°F for 30 minutes and then allowed to cool at room temperature for one hour shall show no evidence of stiffening, softening or cracking of the material.

Workmanship. The complete blood pressure sound chamber and cuff unit shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One sound chamber and cuff unit of the size specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Inspection level shall be S-1. AQL shall be 1 and acceptance number shall be zero.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers, Sizes and their respective Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	SIZE
6515-00-420-5749	SOUND CHAMBER AND CUFF, BLOOD PRESSURE, Adult	I
6515-00-435-8961	SOUND CHAMBER AND CUFF, BLOOD PRESSURE, MEDIUM, Adult	II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5468
Location: c:\word\doc\tarun\sounacid\db

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

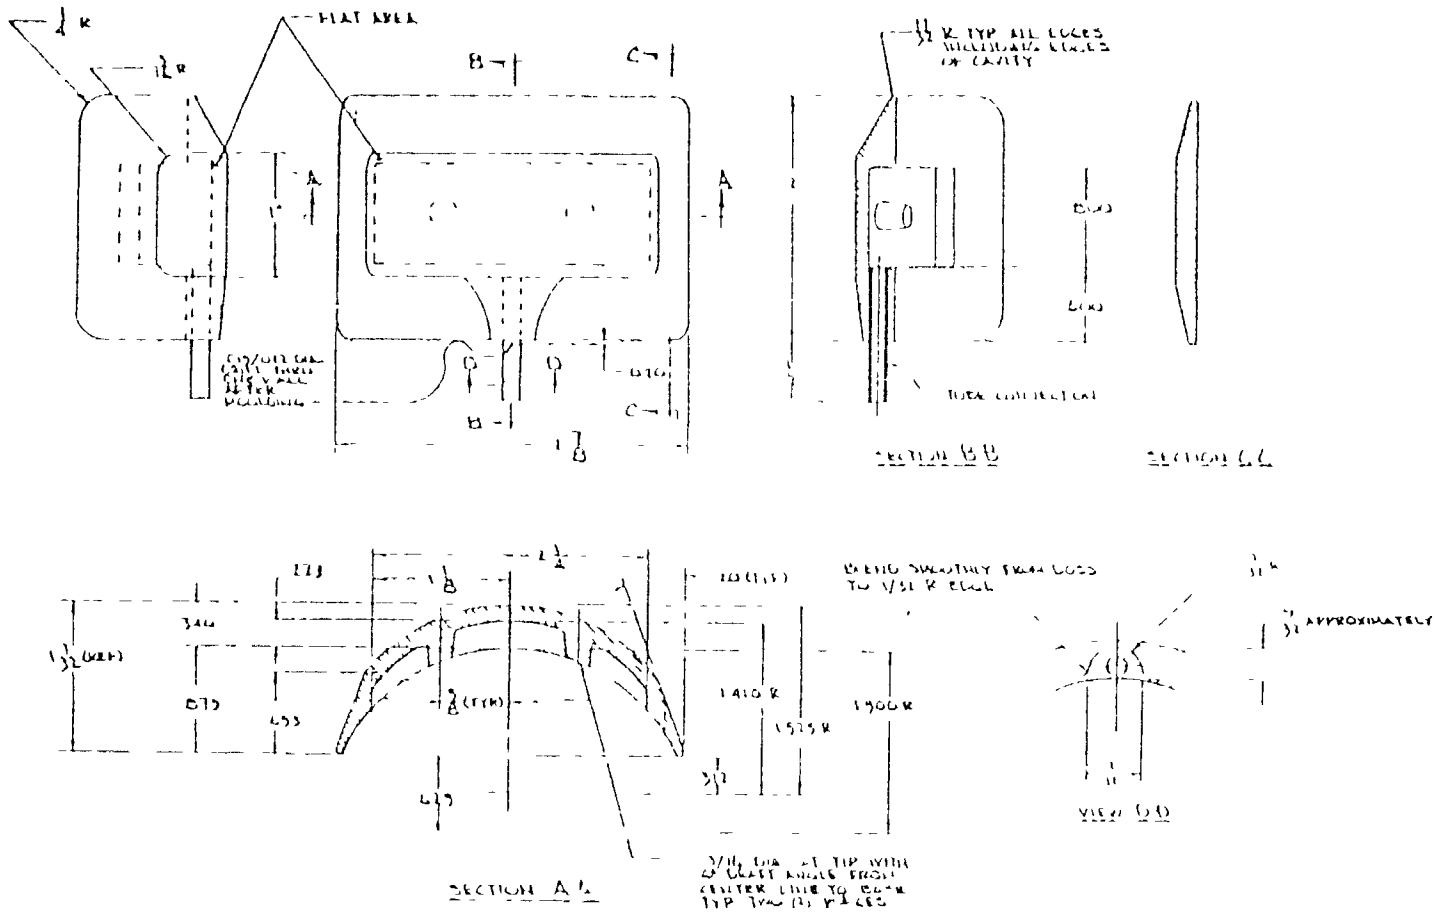

NOTE

ALL EDGES MUST BE FREE FROM TEARS & FLASH.


NSN 6515-00-455 8961

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 10%	± 10%	± 10%

A-A-54895

FIGURE 1-A SOUND CHAMBER & CUFF, BLOOD PRESSURE (MEDIUM ADULT)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

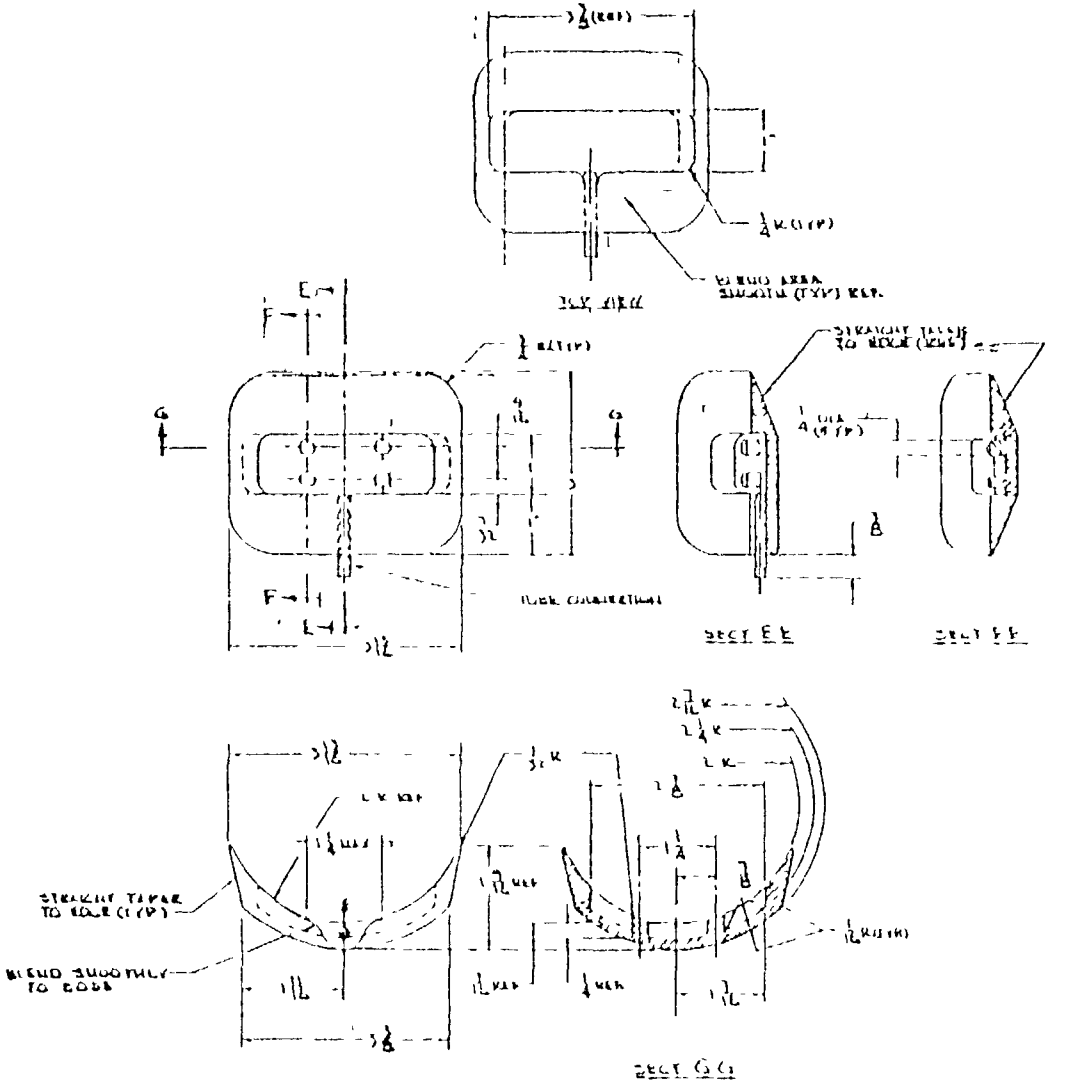

NOTE
ALL EDGES MUST BE FREE FROM TEARS & FLASH.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 10%	± 10%	± 10%

NSN 6515-00-420-5749

FIGURE 1-B SOUND CHAMBER & CUFF, BLOOD PRESSURE (ADULT)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54895	2 DOCUMENT DATE (YYMMDD) 930716

3 DOCUMENT TITLE
SOUND CHAMBER AND CUFF, BLOOD PRESSURE

4 NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.*)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (*Last, First, Middle Initial*)	b ORGANIZATION
c ADDRESS (*Include Zip Code*)	d TELEPHONE (*Include Area Code*) (1) Commercial (2) AUTOVON (*If applicable*)
	e DATE SUBMITTED (*YYMMDD*)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: DPSC-MSE	b TELEPHONE (*Include Area Code*) (1) Commercial: (215)7372870 (2) AUTOVON: 444-2870
c ADDRESS (*Include Zip Code*) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — *Previous editions are obsolete* — 198/29

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.