INCH-POUND

A-A-54899

31 August 1993

# COMMERCIAL ITEM DESCRIPTION

## SPONGE, SURGICAL, GAUZE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-37172 which is cancelled.

This Commercial Item Description covers a non-sterile, pre-washed absorbent gauze sponge.

Salient characteristics:

Shall be a non-sterile, pre-washed absorbent gauze sponge, suitable for use as a surgical preparation, for cleansing wounds or as a post-surgical dressing.

The gauze material shall be Type A or Type B as indicated herein.

AMSC N/A FSC 6510

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Type A. Cotton threads shall be woven into an open fabric with selvaged edges. The fabric shall be bleached white. The gauze shall be treated with caustic, bleached, and then slack laundered so that it has excess crimp in both the warp and filling direction, resulting in a finished structure so that one layer will cling to an under layer. Material shall have a nominal unstretched width of 27 inches. The finished material shall meet the requirements of the Pharmacopoeia of the United States (U.S.P.), except that the thread count shall be minimum of 8 in the filling and minimum of 12 in the wrap

Type B. Gauze used shall be Type VII gauze, in accordance with the U.S.P.

Construction with Type A gauze. The gauze material shall be cut into 16 inch lengths. Cuts shall be at right angles to the selvage edges. The gauze shall be "Z" folded evenly to 3-ply, forming a pad 9 inches wide by 16 inches long. The cut edges shall be folded toward the center, forming a pad 9 inches wide by 8 inches long. Corners of the pad shall then be folded inward, forming a diamond shaped pad with nominal overall dimensions of 6 by 6¾ inches (stretched). Folding shall be as specified in Figure 1.

Construction with Type B gauze. An 18 inch by 16 inch (nominal) rectangle of gauze (288 square inches minimum) shall have the four corners folded inward to slightly overlap. The four folded corners shall be again folded inward to slightly overlap. If necessary, to obtain dimensions of 4 inches minimum by 8 inches maximum, this folding shall be repeated a third time. The finished sponge shall have one side as a continuous gauze surface, the other side shall have folded inward sections.

Workmanship. The sponge shall be free from defects which detract from their appearance or impair their serviceability.

Unit. Package (PG). One package containing six hundred (600)sponges, as specified, constitutes one unit.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 with an AQL of 1.0 (percent defective) and an inspection level of S-3. The unit of product for examination purposes shall be ten sponges.

Sampling for tests. Sampling for tests (dimensional), shall be conducted in accordance with MIL-STD-105, with an AQL of 0 (percent defective and an inspection level of S-1. The unit of product for test purposes shall be ten sponges.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics. The gauze shall be tested for compliance with U.S.P. The thread count shall be as specified herein, as applicable.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

| NSN | ITEM IDENTIFICATION |
|---|---|
| 6510-00-142-8728 | SPONGE, SURGICAL, GAUZE |



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

A-A-54899

MILITARY INTERESTS:

Custodians:

Air Force-03
Army -MD
Navy-MS

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

FDA-MPQAS
USPHS
VA-OSS

Project Number: 6510-0810



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

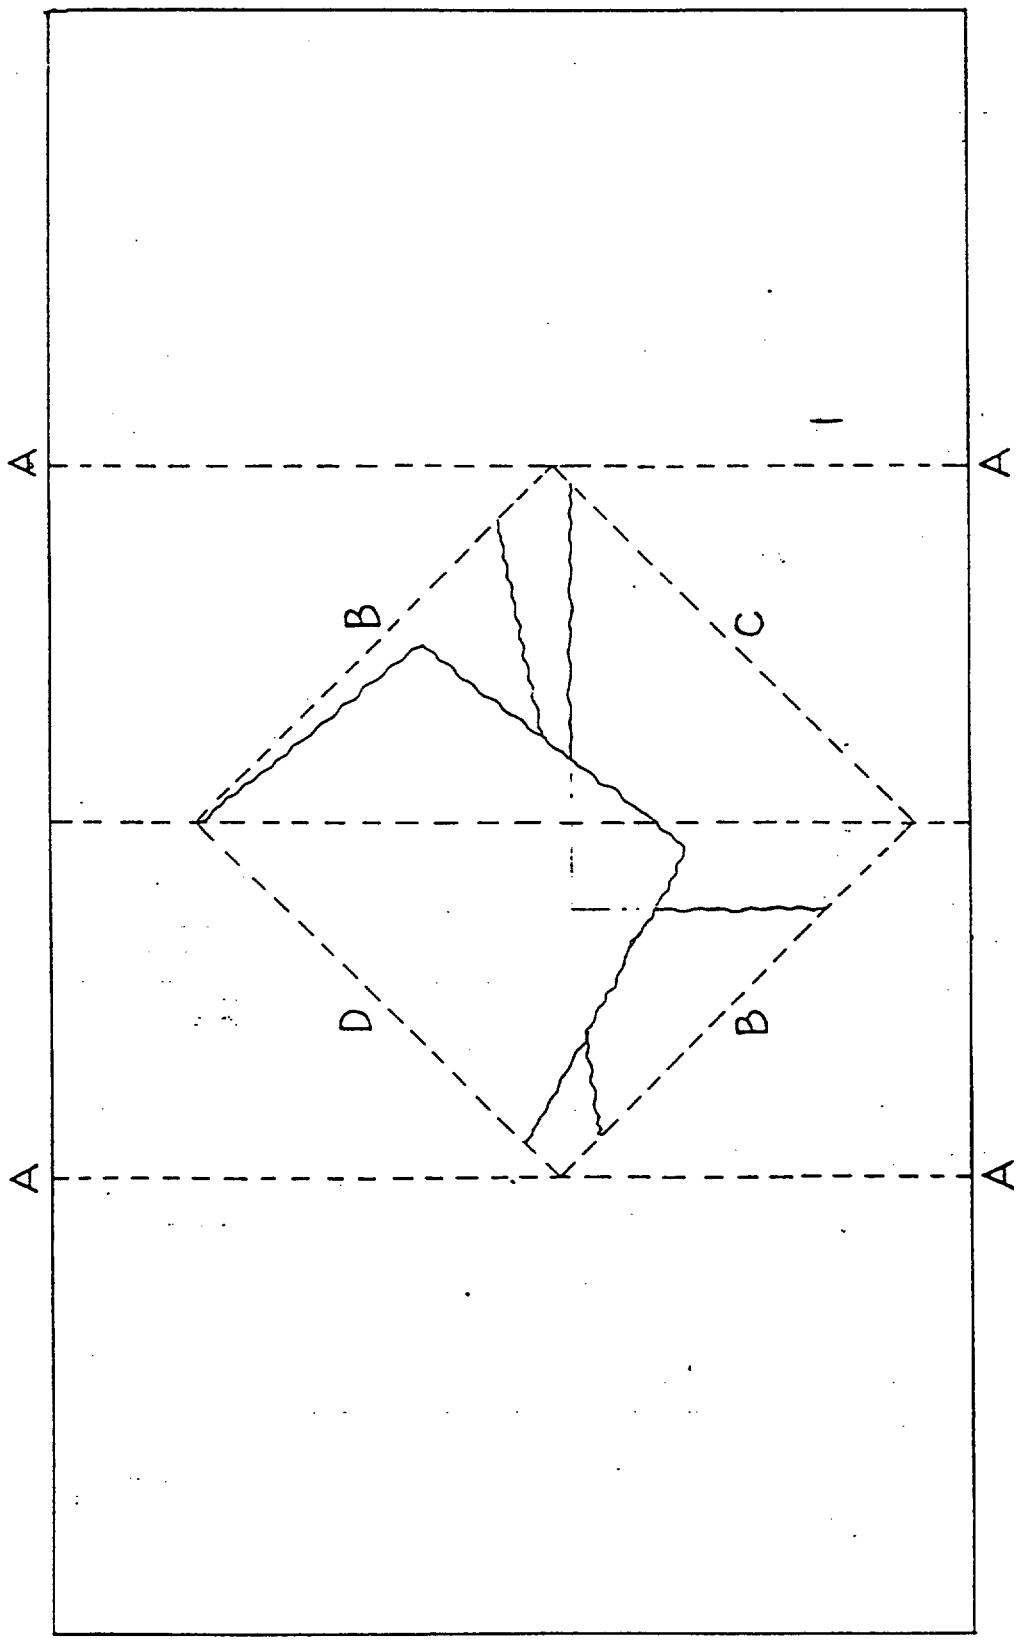


NOTES: 1. DASHED LINES ON DIAGRAM SHOW POSITION OF FOLDS, AND LETTERS REPRESENT ORDER OF FOLDING FLUFFS.
2. LAST FOLD MUST OVERLAP PRECEDING FOLD.

FIG. 1

NSN 6510-00-142-8728



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

## INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

| I RECOMMEND A CHANGE: | 1. DOCUMENT NUMBER | 2. DOCUMENT DATE (YYMMDD) |
|---|---|---|
| | A-A-54899 | 31 August 1993 |

**3. DOCUMENT TITLE**
SPONGE, SURGICAL, GAUZE

**4. NATURE OF CHANGE** *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

**5. REASON FOR RECOMMENDATION**

**6. SUBMITTER**

| a. NAME (Last, First, Middle Initial) | b. ORGANIZATION | |
|---|---|---|
| c. ADDRESS (Include Zip Code) | d. TELEPHONE (Include Area Code)<br>(1) Commercial<br>(2) AUTOVON (If applicable) | 7. DATE SUBMITTED (YYMMDD) |

**8. PREPARING ACTIVITY**

| a. NAME | b. TELEPHONE (Include Area Code) | |
|---|---|---|
| Defense Personnel Support Center | (1) Commercial<br>(215) 737-2870 | (2) AUTOVON<br>444-2870 |
| c. ADDRESS (Include Zip Code)<br>ATTN: MSE<br>2800 S. 20th Street<br>Philadelphia, PA 19145 | IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT:<br>Defense Quality and Standardization Office<br>5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466<br>Telephone (703) 756-2340 AUTOVON 289-2340 | |



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.