INCH-POUND

A-A-54901
30 July 1993

COMMERCIAL ITEM DESCRIPTION

SYRINGE, AIR, DENTAL

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-S-915, which is cancelled.

This Commercial Item Description covers a air syringe and replacement bulb suitable for use in dental operative procedures.

Salient characteristics:

Classification. This specification covers the following types and styles:

Type I	Complete Styles Style I Valve in Nozzle Style II Valve in bulb
Type II	Replacement bulb

Material. The nozzle and valve shall be fabricated from chrome plated brass or corrosion-resistant steel. The bulb shall be fabricated from rubber or other suitable elastomeric material.

Style and design. The syringe shall be designed to provide a directed, concentrated stream of air during dental procedures. The bulb and nozzle shall be easily connected and disconnected and shall form an air-tight seal. The bulb shall have a nominal 2 ounce capacity. The bulb shall be easily compressed and shall return to its original configuration without any permanent distoration.

The syringe shall consist of a bulb, nozzle and a air intake check valve. The style and design shall be in accordance with Figures 1 and 2, both styles are acceptable.

Corrosion resistance. The nozzle shall show no signs of corrosion when tested in accordance with ASTM Designations F1089.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Workmanship. The syringe shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). For Type I, one air syringe as specified, constitutes one unit. For Type II, one replacement bulb, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one syringe as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one syringe. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	TYPE
6520-00-501-8000	SYRINGE, AIR, DENTAL, Bulb	I
6520-00-501-9000	BULB, AIR SYRINGE, DENTAL	II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS
GSA-FSS-FCGC

Project No. 6520-2545
Location: C:\MARK\SYRINGE\D


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

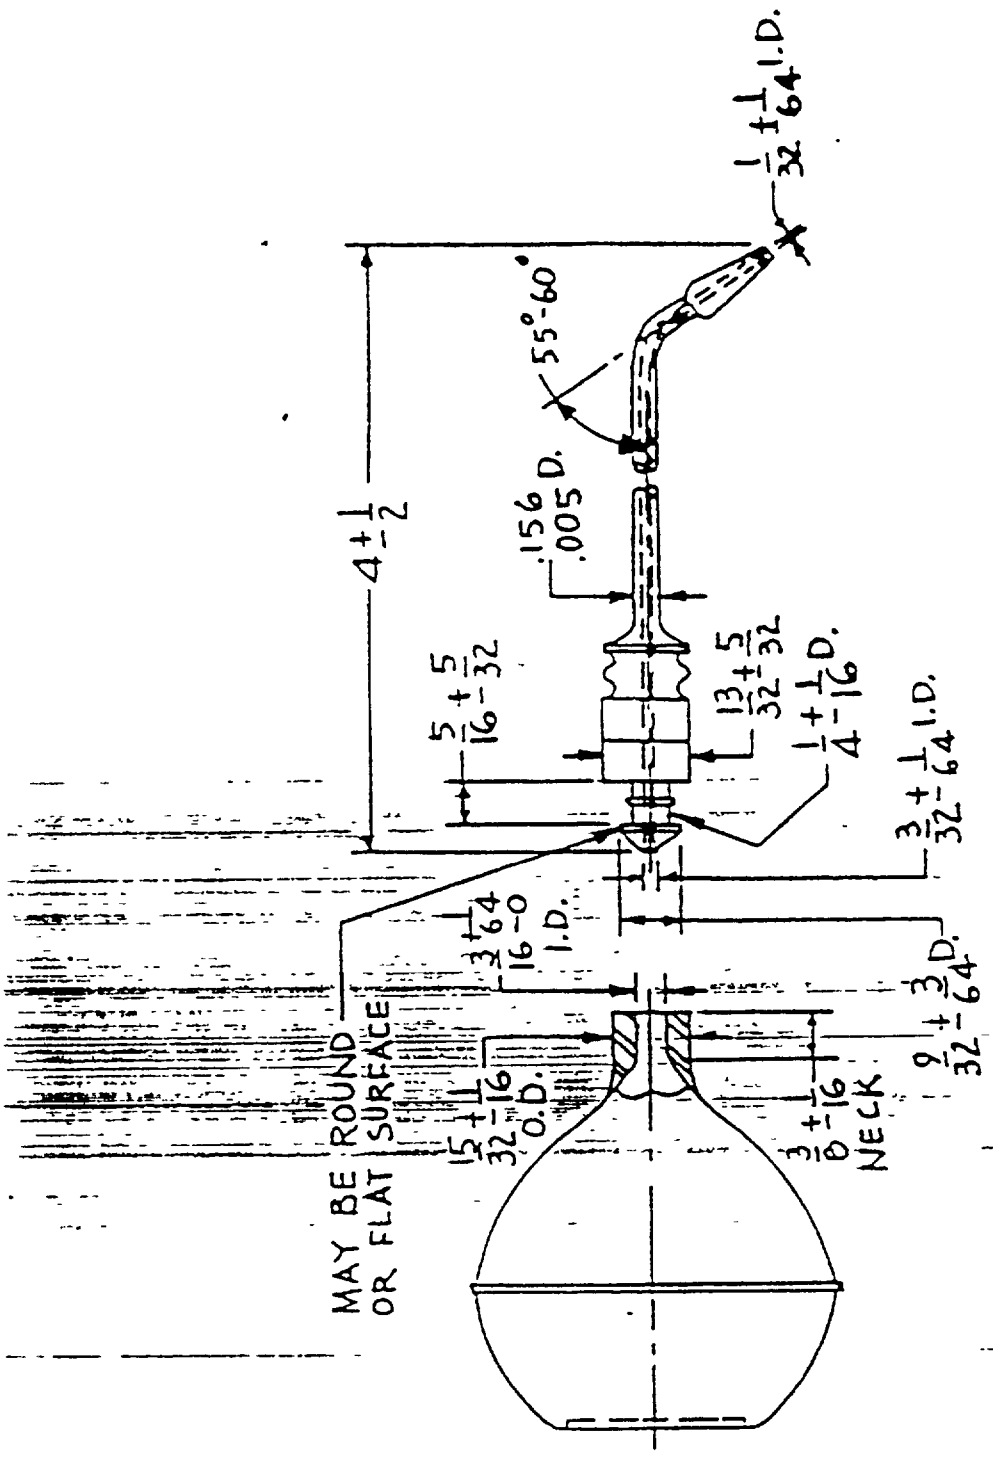

TYPE I, STYLE I
COMPLETE SYRINGE


FIGURE 1. COMPLETE SYRINGE WITH VALVE IN NOZZLE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

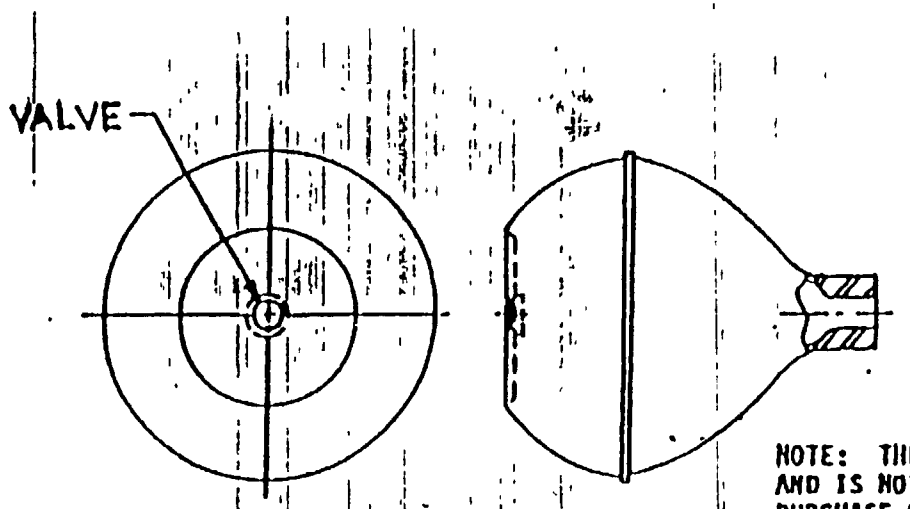

NOTE: THE BULB SHOWN IS TYPICAL IN VALVE PLACEMENT AND IS NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF BULBS AND/OR SYRINGES WHICH ARE OTHERWISE IN ACCORDANCE WITH THE REQUIREMENTS OF THIS DOCUMENT.

TYPE II
REPLACEMENT BULB

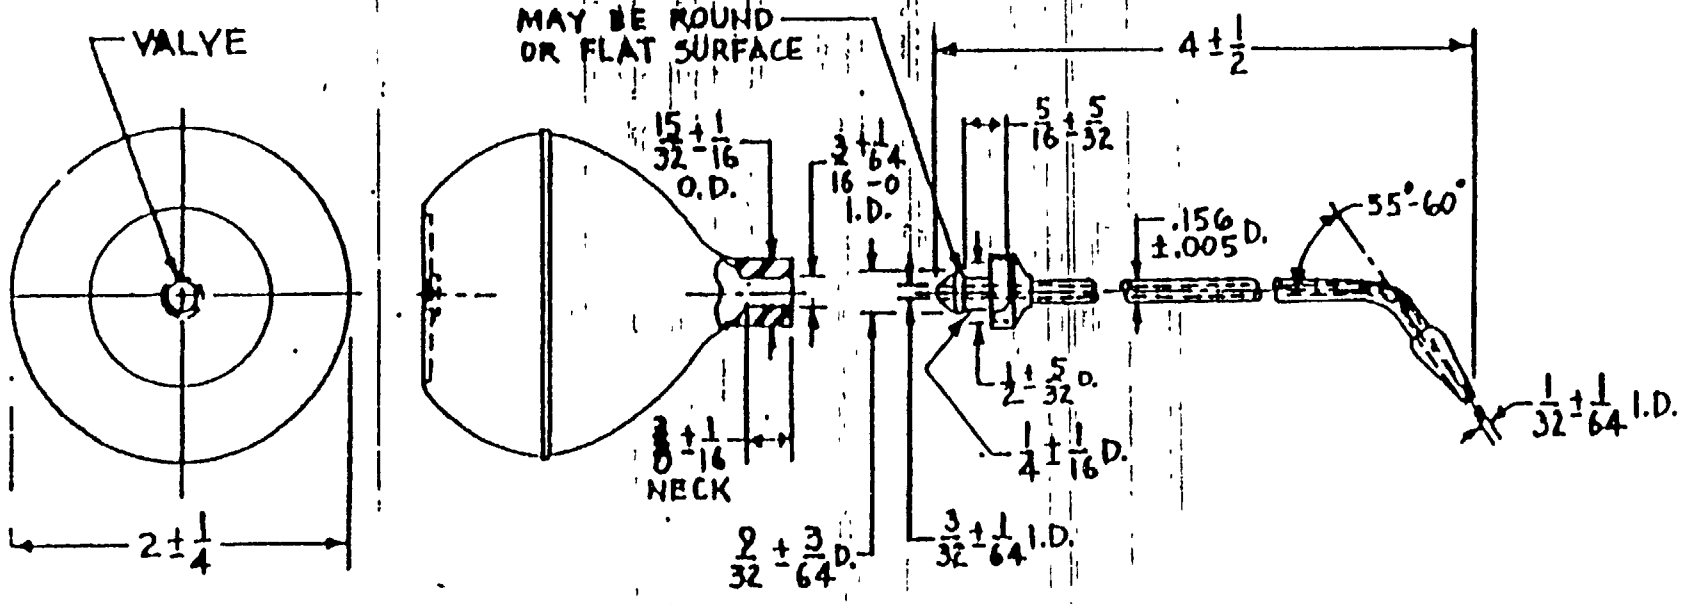

TYPE I, STYLE II
COMPLETE SYRINGE

FIGURE 2. COMPLETE SYRINGE WITH VALVE IN BULB AND REPLACEMENT BULB

A-A-54901

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54901	930730

3. DOCUMENT TITLE
SYRINGE, AIR, DENTAL

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)737-2870	444-2870
c. ADDRESS (Include Zip Code) 2800 South 20TH Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.