INCH-POUND

A-A-54908
31 August 1993

# COMMERCIAL ITEM DESCRIPTION

## CANNULA, BRAIN, (Frazier)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-C-121, which is cancelled.

This Commercial Item Description covers an 8 Fr. angled suction tube of the Frazier design suitable for use in general surgical procedures.

Salient characteristics:

General. The cannula shall consist of the tube, tubing connector with a thumb piece suction control port and a stylet. The cannula tube at the proximal end shall be permanently attached to the tubing connector and have a blunt open tip at the distal end. The tubing connector shall be sized for suction tubing ranging from 1/8 to 3/16 inch inside diameter. The stylet assembly shall consist of a knurled handle or knob and a permanently attached steel wire.

Material. The cannula tube, thumb piece and stylet assembly shall be manufactured from Class 3, austenitic stainless steel in accordance with ASTM Designation F899.

Hardness. The cannula tube, thumb piece and stylet handle shall have a Rockwell Hardness B scale (HRB) of 70 to 95 when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Finish The finish of components shall be mirror or satin.

Style, design and dimensions. Cannulas shall be in accordance with Figure 1.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Passivation. Cannulas shall be properly passivated.

Corrosion resistance. Cannulas shall show no signs of corrosion when tested for corrosion resistance in accordance with ASTM Designation F1089.

Identification marking and labeling. Cannulas shall be legibly marked with the contractor's name or registered trademark and shall also have the word "stainless" marked on the thumb piece Cannulas of foreign manufacture shall bear the name of the country of origin.

Workmanship. The cannula and stylet assembly shall be uniform and free from cracks, pits, burrs, sharp edges, scale, rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Visual and dimensional examination. Cannula and stylet assembly shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements.

Unit. Each (EA). One cannula, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one cannula as specified. Sampling shall be general inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one cannula. Sampling shall be special inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 202640-26T09:40Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.



Source: https://assist.dla.mil -- Downloaded: 202640-26T09:40Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

| NATIONAL STOCK NUMBER | ITEM IDENTIFICATION |
|---|---|
| 6515-00-386-6800 | CANNULA, BRAIN, Frazier, 8 Fr., Angular, 5-5/8 inch (14.3 cm) Long |

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS
GSA-FSS-FCGC

Project Number: 6515-5619
Location: c:\word\doc\david\cannula2\sg



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

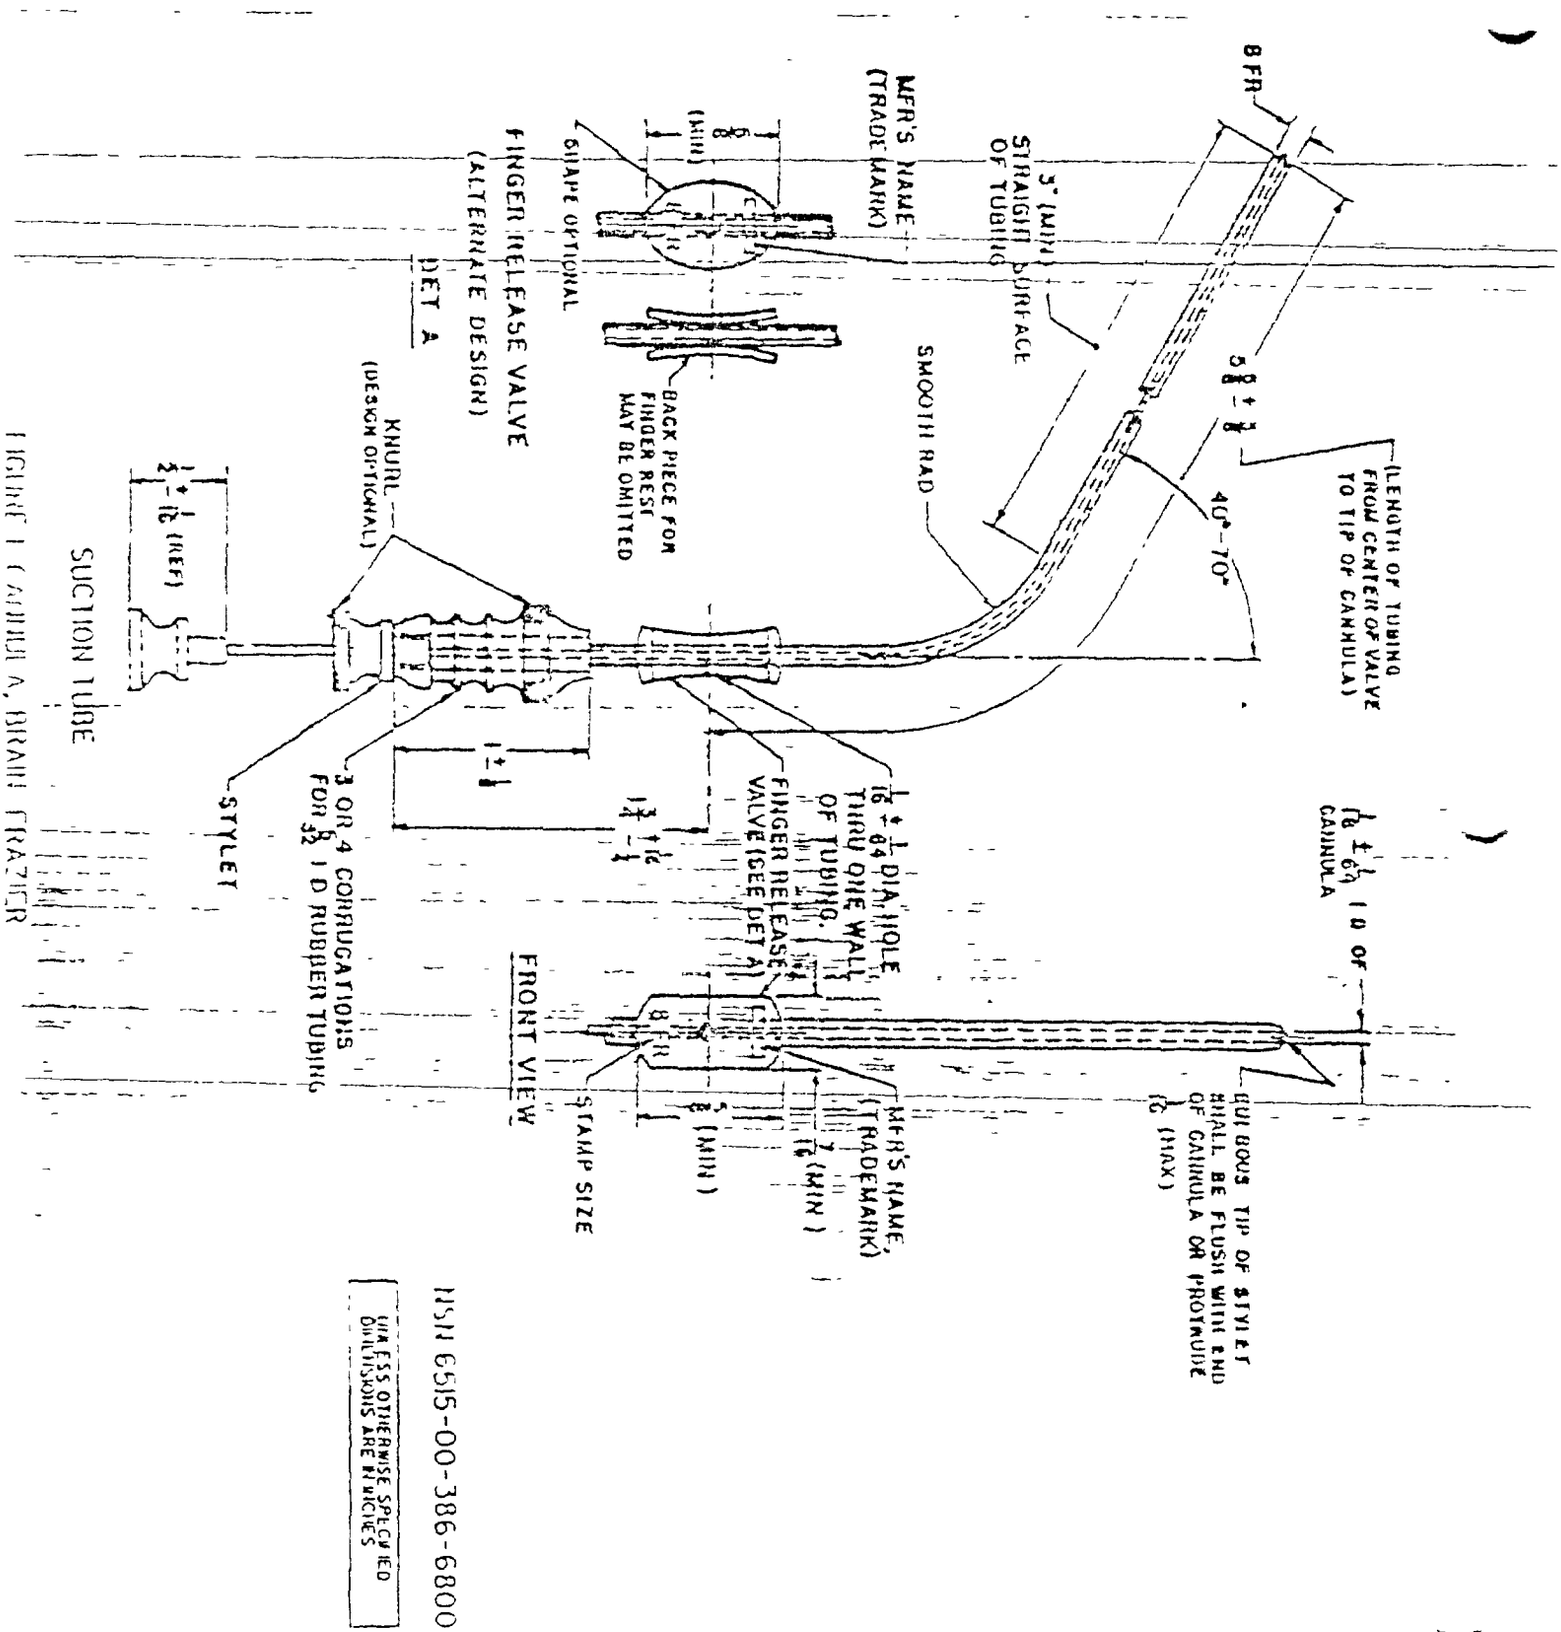



FIGURE 1. Cannula, Brain Frazier

NSN 6515-00-386-6800



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

## INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

| I RECOMMEND A CHANGE: | 1. DOCUMENT NUMBER<br>2-A-54908 | 2. DOCUMENT DATE (YYMMDD)<br>930831 |
|---|---|---|

3. DOCUMENT TITLE
CANNULA BRAIN (Frazier)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

| a. NAME (Last, First, Middle Initial) | b. ORGANIZATION | |
|---|---|---|
| c. ADDRESS (Include Zip Code) | d. TELEPHONE (Include Area Code)<br>(1) Commercial<br>(2) AUTOVON<br>(If applicable) | 7. DATE SUBMITTED (YYMMDD) |

8. PREPARING ACTIVITY

| a. NAME | b. TELEPHONE (Include Area Code) | |
|---|---|---|
| Defense Personnel Support Center<br>ATTN: DPSC-MSE | (1) Commercial<br>(215)7372870 | (2) AUTOVON<br>444-2870 |
| c. ADDRESS (Include Zip Code)<br>2800 South 20th Street<br>Philadelphia, PA 19145 | IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT:<br>Defense Quality and Standardization Office<br>5203 Leesburg Pike Suite 1403 Falls Church, VA 22041 3466<br>Telephone (703) 756-2340 AUTOVON 289-2340 | |



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.