INCH-POUND
A-A-54909
3 September 1993

# COMMERCIAL ITEM DESCRIPTION

## CURETTE, MASTOID, Spratt

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-C-1969A, which is cancelled.

This Commercial Item Description covers mastoid curettes of the Spratt design suitable for excision of mastoid cells during the mastoid process.

Salient characteristics:

General. Curettes shall have oval shaped cups which have a sharp edge and be of the following sizes:

Size 00
Size 1
Size 2
Size 3
Size 5
Size 6

Material. The material shall be Class 4 stainless steel, as an alternate the handle shall be Class 3 stainless steel, in accordance with American Society for Testing and Materials (ASTM) F899.

Style, design and dimensions. Curettes shall be in accordance with Figure 1 for style, design and dimensions.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:40Z
Check the source to verify that this is the current version before use.

Hardness. Curettes shall have a Rockwell Hardness C scale (HRC) of 45 to 53 for the shank and cup, shanks of Class 3 stainless steel shall have a minimum HRB of 85, when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Finish. The finish of the curettes shall be mirror, satin or matte. The matte finish shall exhibit a uniform nondirectional surface texture equivalent to that produced by lightly blasting the prepared surface with fine abrasives under pressure.

Passivation. Curettes shall be properly passivated.

Corrosion resistance. Curettes shall show no signs of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM Designation F1089.

Identification marking and labeling. Curettes shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Curettes of foreign manufacture shall bear the name of the country of origin.

Workmanship. Curettes shall be uniform and free from cracks, pits, burrs, sharp edges, scale, rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Unit. Each (EA). One curette, of the size specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one curette. Sampling shall be general inspection level S-2 with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one curette. Sampling shall be special inspection level S-2 with an AQL of 1.0.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

| NATIONAL STOCK NUMBER | ITEM IDENTIFICATION | SIZE |
|---|---|---|
| 6515-00-322-5400 | CURETTE, MASTOID, Spratt | 00 |
| 6515-00-322-5500 | CURETTE, MASTOID, Spratt | 1 |
| 6515-00-322-5550 | CURETTE, MASTOID, Spratt | 2 |
| 6515-00-322-5600 | CURETTE, MASTOID, Spratt | 3 |
| 6515-00-322-5700 | CURETTE, MASTOID, Spratt | 5 |
| 6515-00-322-5750 | CURETTE, MASTOID, Spratt | 6 |

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

A-A-54909


CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS
GSA-FSS-FCGC

Project Number: 6515-5618
Location: Intergraph/Curette




Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

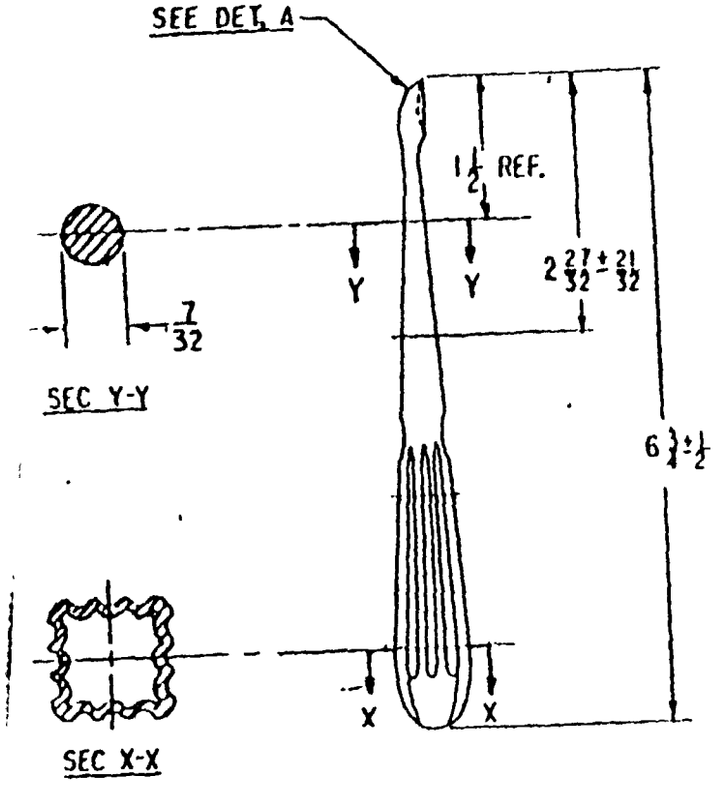

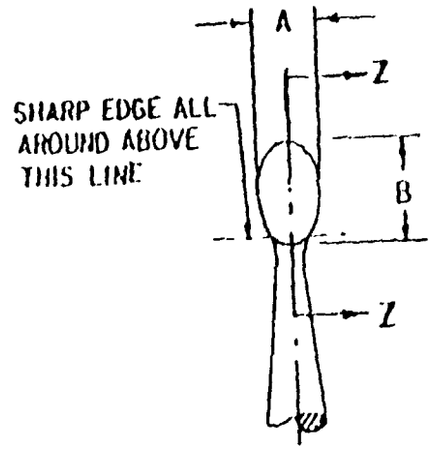
DET. A




SECT Z-Z

| NSN | SIZE | A | B | C | D |
|---|---|---|---|---|---|
| 6515-00-322-5400 | 00 | 1/8 | 15/64 | 3/32 | 3 ± 1 / 64 64 |
| 6515-00-322-5500 | 1 | 5/32 | 1/4 | 3/32 | 3 ± 1 / 64 64 |
| 6515-00-322-5550 | 2 | 13/64 | 19/64 ± 1/16 | 5/32 ± 1/16 | 1/16 ± 1/64 |
| 6515-00-322-5600 | 3 | 9/32 | 13/32 ± 1/16 | 11/64 ± 3/64 | 3/32 ± 1/64 |
| 6515-00-322-5700 | 5 | 9/32 | 15/32 | 3/16 | 3 ± 1 / 64 64 |
| 6515-00-322-5750 | 6 | 3/8 | 17/32 ± 1/16 | 7/32 ± 1/16 | 7/64 ± 3/64 |

UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES.

FIGURE 1 CURETTE, MASTOID, SPRATT

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

## INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE. This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

| I RECOMMEND A CHANGE: | 1. DOCUMENT NUMBER<br>A-A-54909 | 2. DOCUMENT DATE (YYMMDD)<br>930903 |
|---|---|---|

3. DOCUMENT TITLE
CURETTE, MASTOID, Spratt

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

| a. NAME (Last, First, Middle Initial) | b. ORGANIZATION | |
|---|---|---|
| c. ADDRESS (Include Zip Code) | d. TELEPHONE (Include Area Code)<br>(1) Commercial<br>(2) AUTOVON (If applicable) | 7. DATE SUBMITTED (YYMMDD) |

8. PREPARING ACTIVITY

| a. NAME<br>Defense Personnel Support Center<br>ATTN: DPSC-MSE | b. TELEPHONE (Include Area Code)<br>(1) Commercial: (215)737-2870<br>(2) AUTOVON: 444-2870 |
|---|---|
| c. ADDRESS (Include Zip Code)<br>2800 South 20th Street<br>Philadelphia, PA 19145 | IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT:<br>Defense Quality and Standardization Office<br>5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466<br>Telephone (703) 756-2340 AUTOVON 289-2340 |

DD Form 1426, OCT 89 — Previous editions are obsolete.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.