INCH-POUND

A-A-54910

3 September 1993

COMMERCIAL ITEM DESCRIPTION

RONGEUR, Stille, 9 inch

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers both curved and straight, double action Stille rongeurs suitable for bone removal during surgical procedures.

Salient characteristics:

General. Rongeurs shall be double action, self opening via a spring in the handle and of the Stille design suitable for removal of bone during surgical procedures.

Material. The material shall be Class 4 stainless steel except for the spring which may be Class 3 stainless steel in accordance with ASTM F899.

Style, design and dimensions. Rongeurs shall be in accordance with Figures 1 and 2 for style, design and dimensions.

Hardness. Rongeur jaws shall have a Rockwell Hardness C scale (HRC) of 48 to 55, handles HRC 45 minimum, screws, pins and rollers HRC 36 minimum, and spring HRC of 38 to 45 except for springs made from Class 3 stainless steel which shall have a HRC of 20 minimum when tested in accordance with American Society for Testing and Materials (ASTM) Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Finish. The finish of the instrument shall be mirror, satin, or mirror and satin.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Identification marking. Rongeur's shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Rongeurs of foreign manufacture shall bear the name of the country of origin.

Workmanship. Rongeurs shall be uniform and free from cracks, pits, burrs, sharp edges, scale, rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Unit. Each (EA). One rongeur as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as specified. Unit of product for examination purposes shall be one Stille rongeur. Sampling shall be general inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one rongeur. Sampling shall be special inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-331-4800	RONGEUR, Curved, Stille, 9 inch
6515-00-331-5400	RONGEUR, Straight, Stille-Luer, 9 inch

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5650
Location: Intergraph/Rongeur


Source: https://assist.dla.mil -- Downloaded: 202610-26T09:40Z
Check the source to verify that this is the current version before use.

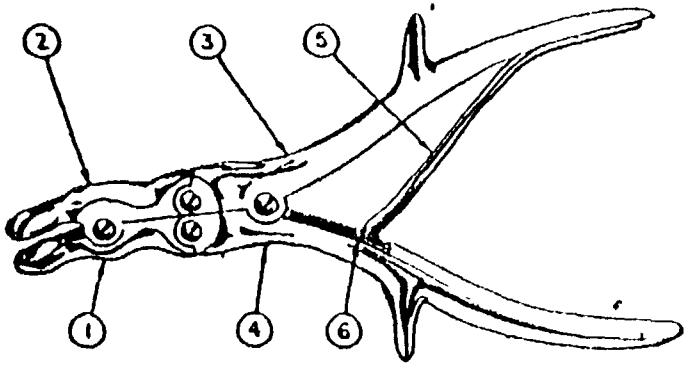


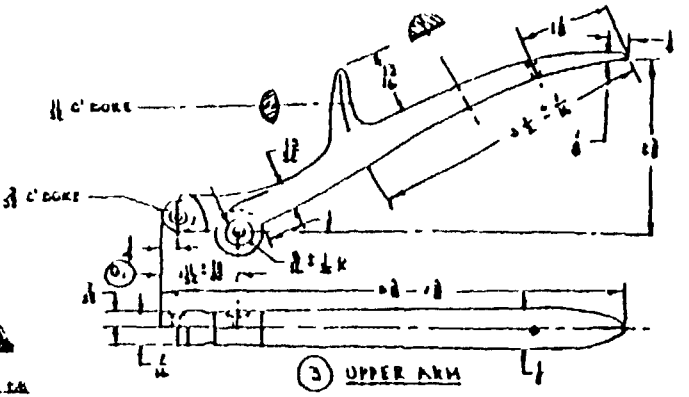





VIEW C-C

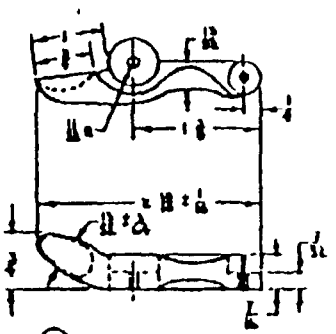


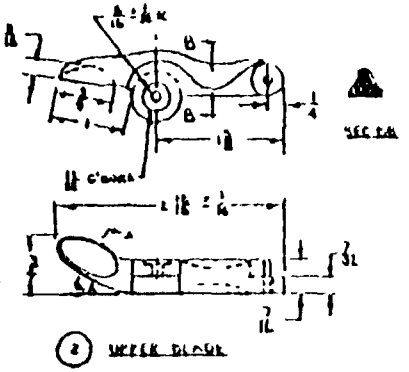


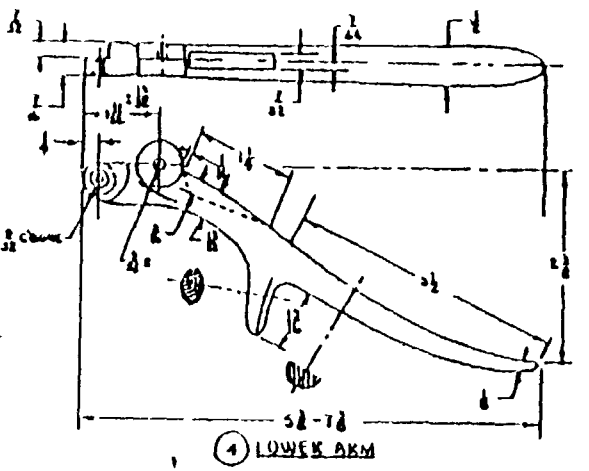


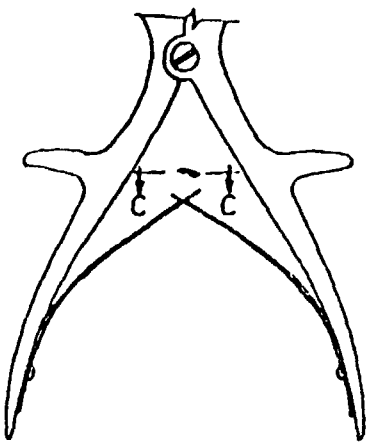

ALTERNATE SPRING DESIGN

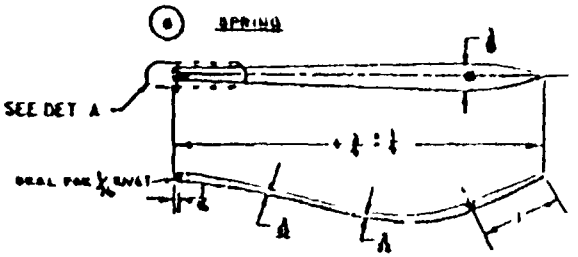





DETAIL A

GENERAL NOTES:

1. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.


UNLESS OTHERWISE SPECIFIED TOLERANCE SHALL BE:

UP TO 1/4 INCH	±1/64 INCH
OVER 1/4 INCH TO 1/2 INCH	±1/32 INCH
OVER 1/2 INCH TO 1 INCH	±1/16 INCH
OVER 1 INCH	±1/8 INCH

NSN 6515-00-331-4800

FIGURE 1 RONGEUR, CURVED, STILLE, 9 INCH

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:40Z
Check the source to verify that this is the current version before use.

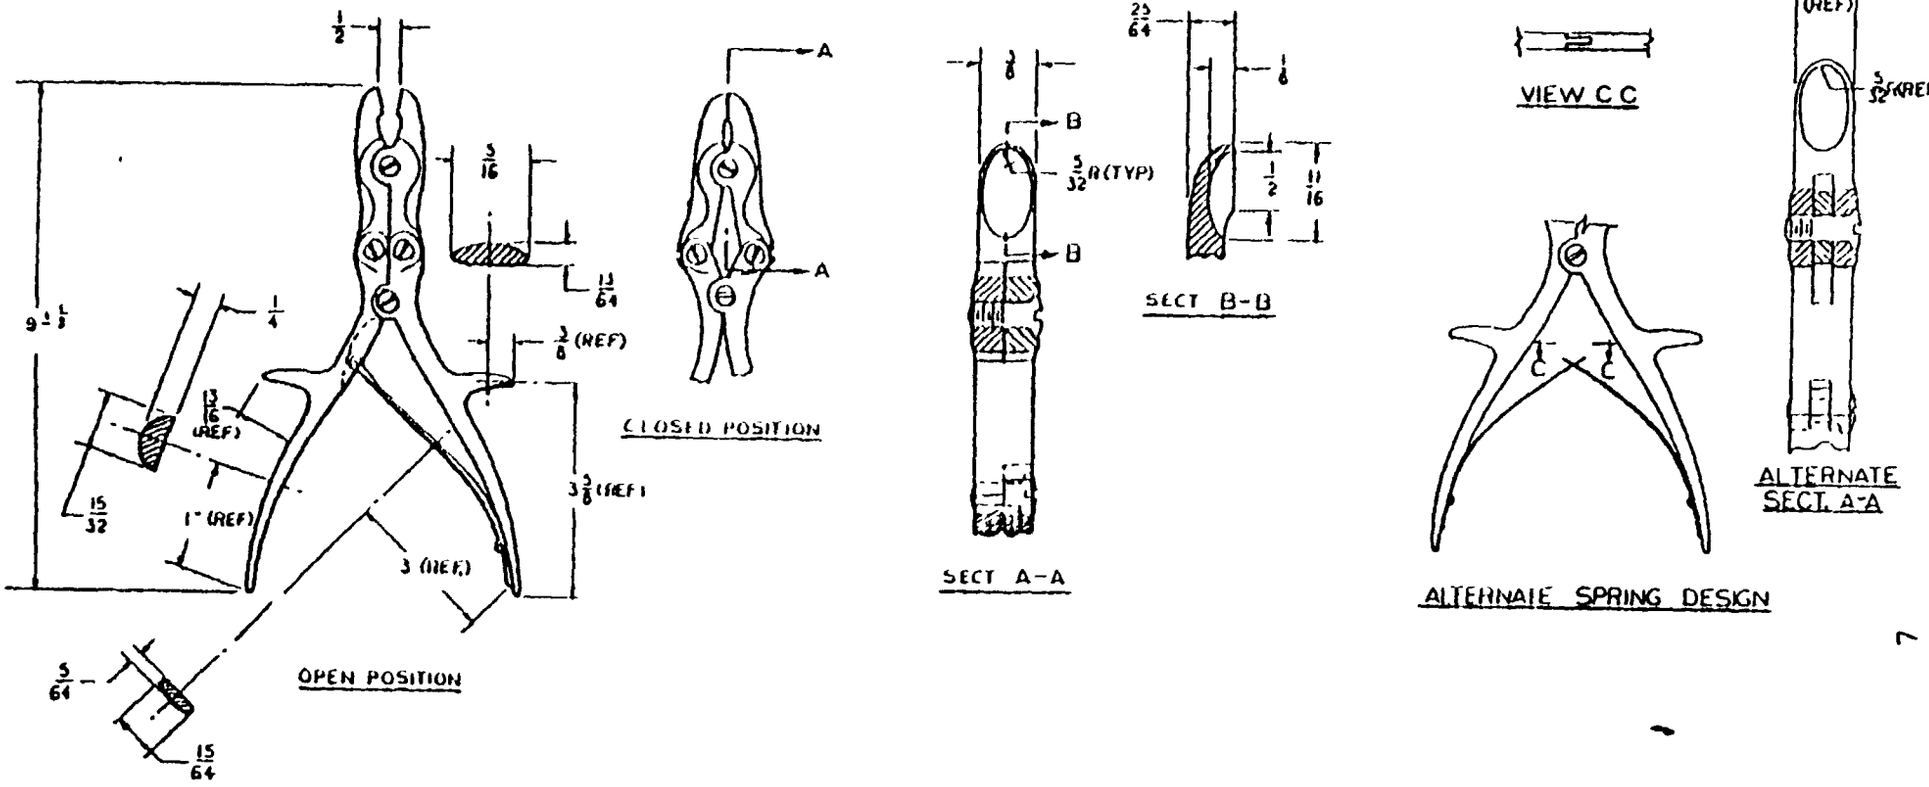

NOTES:

1. ALL DIMENSIONS IN INCHES.
2. UNLESS OTHERWISE SPECIFIED TOLERANCES SHALL BE:

   1/8 INCH & UNDER ±1/64
   OVER 1/8 TO 1/2 INCH ±1/32
   OVER 1/2 INCH ±1/8

3. NSN 6515-00-331-5400

FIGURE 2. HEMOSTAT, STRAIGHT, STILLE LUER, 9 INCH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54910	2 DOCUMENT DATE (YYMMDD) 930903

3 DOCUMENT TITLE
RONGEUR, Stille, 9 inch

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: DPSC-MSE	b TELEPHONE (Include Area Code) (1) Commercial: 215-737-2870 (2) AUTOVON: 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 198/29

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.