INCH-POUND

A-A-54917
19 November 1993

COMMERCIAL ITEM DESCRIPTION

BRUSH, SURGICAL SCRUB

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specification GG-B-2043, which is cancelled.

This Commercial Item Description covers surgical scrub brushes.

Salient characteristics:

Classification. The brushes shall be of the following styles:

Style A - Rectangular shaped handle
Style B - U-shaped handle

Material. The bristles shall be fabricated from black nylon. The block shall be fabricated from rigid plastic. The anchor pins shall be fabricated from corrosion resistant metal.

Style and design. Each brush shall consist of a block, bristles and anchor pins. The block shall be white. The block for Style A shall be solid or hollow. The block for the Style B brush shall be channeled or U-shaped.

The bristles shall be 0.010 ± 0.001 inch in diameter. The face of the brush shall consist of seven horizontal rows with a minimum of 16 tufts per row. Each tuft shall contain a minimum of 54 bristles and shall be securely embedded in the block with an anchor pin. The Style and design shall be in accordance with Figures 1 and 2.

Identification markings. Each brush shall be marked with the name or registered trademark of the manufacturer.

AMSC N/A FSC 6530
DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Finish. The block shall have a smooth bright finish.

Workmanship. The brush shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One brush of the style specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one surgical scrub brush as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one surgical scrub brush. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers, Item Identifications and their respective Styles are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION	STYLE
6530-00-044-4820	BRUSH, SURGICAL SCRUB, U-Shaped Handle	B
6530-00-772-5935	BRUSH, SURGICAL SCRUB,	A

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS
GSA-FSS-FCGC

Project Number: 6530-2421
Location: c:\word\doc\levin\brushcid\sg

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

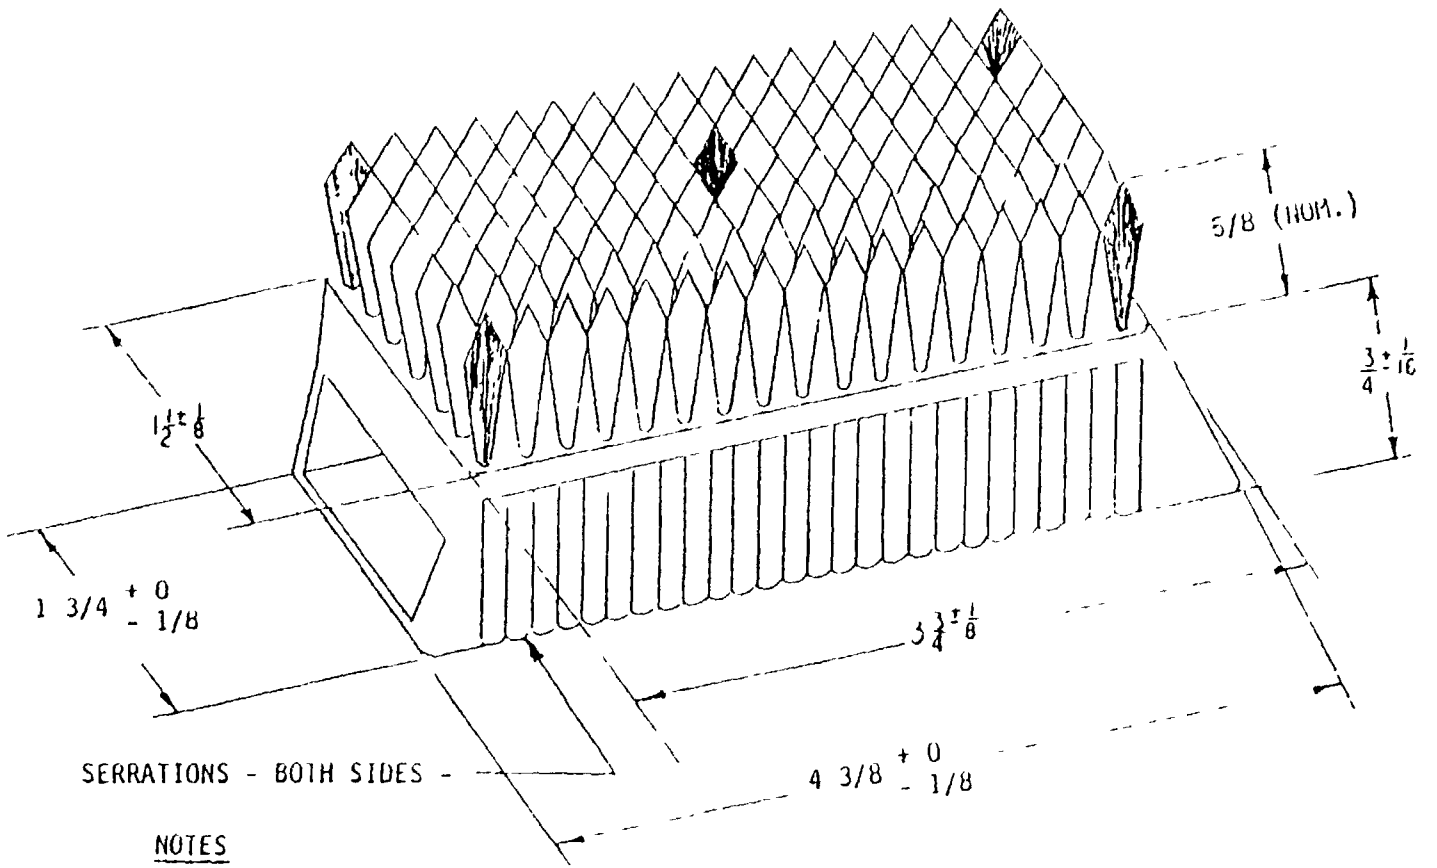


NOTES

1. ALL DIMENSIONS ARE IN INCHES
2. NUMBER AND STYLE OF BRISTLES ARE FOR ILLUSTRATION ONLY.
3 SEE BODY OF THIS SPECIFICATION FOR REQUIREMENTS.

NSN 6530-00-772-5935

FIGURE 1 Brush, Surgical Scrub - Style A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

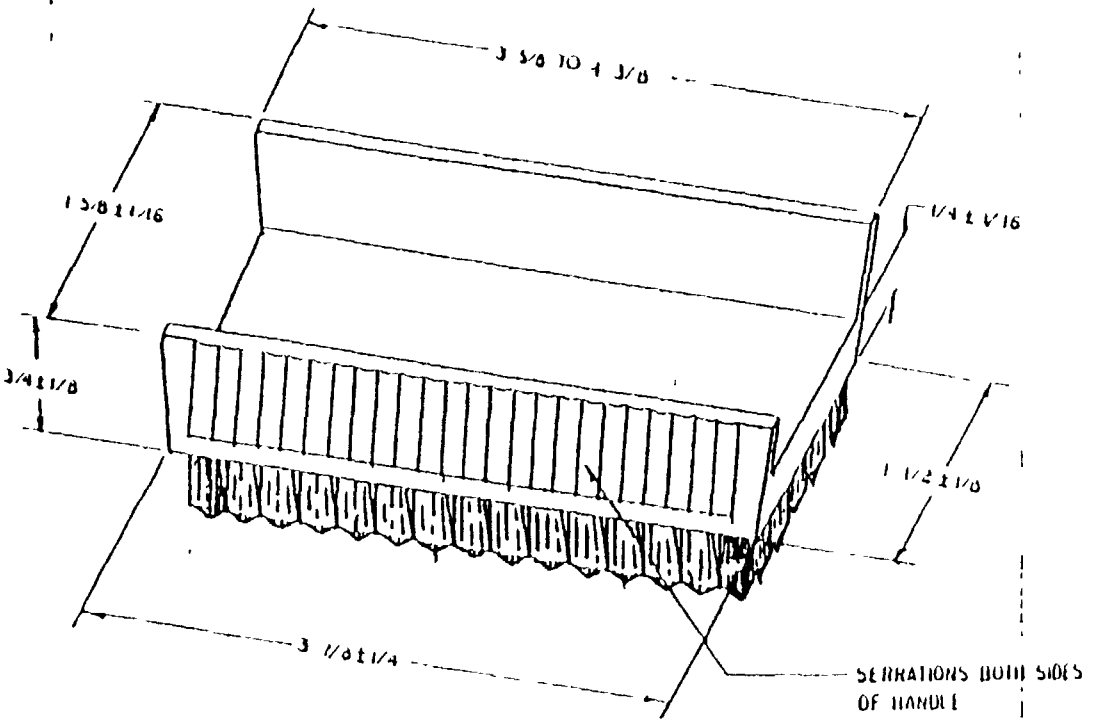

NOTES.

1 ALL DIMENSIONS ARE IN INCHES
2. NUMBER AND STYLE OF BRISTLES ARE FOR ILLUSTRATION ONLY
3 SEE BODY OF THIS SPECIFICATION FOR REQUIREMENTS

NSN 6530-00 044-4820

FIGURE 2 BRUSH, SURGICAL SCRUB - STYLE B

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54927	2 DOCUMENT DATE (YYMMDD) 931110

3 DOCUMENT TITLE

BRUSH, SURGICAL, SCRUB

4 NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed*)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
ADDRESS (Include Zip Code)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT. Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.