INCH-POUND

A-A-54922
8 October 1993

COMMERCIAL ITEM DESCRIPTION

SYRINGE, CARTRIDGE, ASPIRATING

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-37607, which is cancelled.

This Commercial Item Description covers an aspirating type syringe suitable for use with local anesthetic solutions.

Salient characteristics:

Material. The harpoon and piston assembly shall be fabricated from Class 3 austenitic stainless steel in accordance with ASTM F899. All other components shall be fabricated from Class 3 austenitic stainless steel or chromium plated or nickel plated cooper-zinc alloy.

Hardness. All components fabricated from stainless steel shall have a Rockwell hardness of B90 to B100 when tested in accordance with ASTM E18 or ASTM E92.

Style and design. The syringe shall be of the aspirating type designed for use with disposable needles. The syringe shall be of the side loading type for use with 1.8 milliliter (ml) cartridges having an outside diameter of 8.25 to 9.1 millimeters (mm) and an overall length of 63 to 63.5 mm. (See notes). The syringe shall consist of a barrel, thumb ring, finger grip, spring, guide bearing, plunger with harpoon and an adapter.

The adapter shall be furnished with a male thread suitable for securing disposable needles and shall have a 0.028 to 0.032 inch diameter hole at the center to accommodate a 25 gauge cartridge needle.(See notes). The harpoon shall be suitable for engaging the rubber piston of a glass anesthetic solution cartridge.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

The entire syringe shall be autoclavable. The style and design shall be in accordance with Figure 1. One spare harpoon shall be supplied with each syringe.

Corrosion resistance. The syringe shall show no evidence of corrosion when tested in accordance with ASTM 1089.

Performance. A cartridge shall be inserted into a syringe with an attached needle in accordance with the manufacturer's instructions. The rubber plunger of the cartridge shall be pierced by the harpoon and the plunger pushed forward for a distance of 1/2 inch. The plunger shall then be pulled in the opposite direction as in aspiration. The harpoon shall not become disengaged from the cartridge.

Instructions. Each syringe shall contain adequate instructions for the use of the syringe.

Identification marking. Each syringe shall be permanently marked with the name or registered trademark of the manufacturer.

Workmanship. The syringe shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One syringe along with instructions for use, and one replacement plunger with harpoon as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one syringe as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one syringe. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

NOTE 1: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-01-010-8761	SYRINGE, CARTRIDGE, ASPIRATING, THUMB RING HANDLE

NOTE 2: The syringe covered by this specification is suitable for use with the following items in the Federal Supply Catalog:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6505-01-146-7793	LIDOCAINE HYDROCHLORIDE INJECTION, MODIFIED, 2 Percent, with Epinephrine 1, Cartridges, 1.8 ml, 50s
6505-01-362-8317	LIDOCAINE HYDROCHLORIDE INJECTION, USP, 2.0 percent, with Epinephrine 1:100,000 Cartridges, 1.8 ml, 100s
6505-00-823-7942	MEPIVACAINE HYDROCHLORIDE AND LEVONORDEFRIN INJECTION, NF, 2 percent, 1.8 ml, 50s
6505-01-242-9149	MEPIVACAINE HYDROCHLORIDE INJECTION, USP, 3 percent, 1.8 ml, 100
6515-00-181-7403	NEEDLE, HYPODERMIC, CARTRIDGE TYPE, Disposable, 25 Gauge, 13/16 inch, 100s
6515-00-181-7404	NEEDLE, HYPODERMIC, CARTRIDGE TYPE, Disposable, 25 Gauge, 1-3/8 inches, 100s
6515-00-181-7412	NEEDLE, HYPODERMIC, CARTRIDGE TYPE, Disposable, 27 Gauge, 1-3/8 inches, 100s
6515-00-181-7425	NEEDLE, HYPODERMIC, CARTRIDGE TYPE, Disposable, 27 Gauge, 13/16 inch, 100s

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS


Project Number: 6515-5420
Location: c:\word\doc\levin\syringe3\sg


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

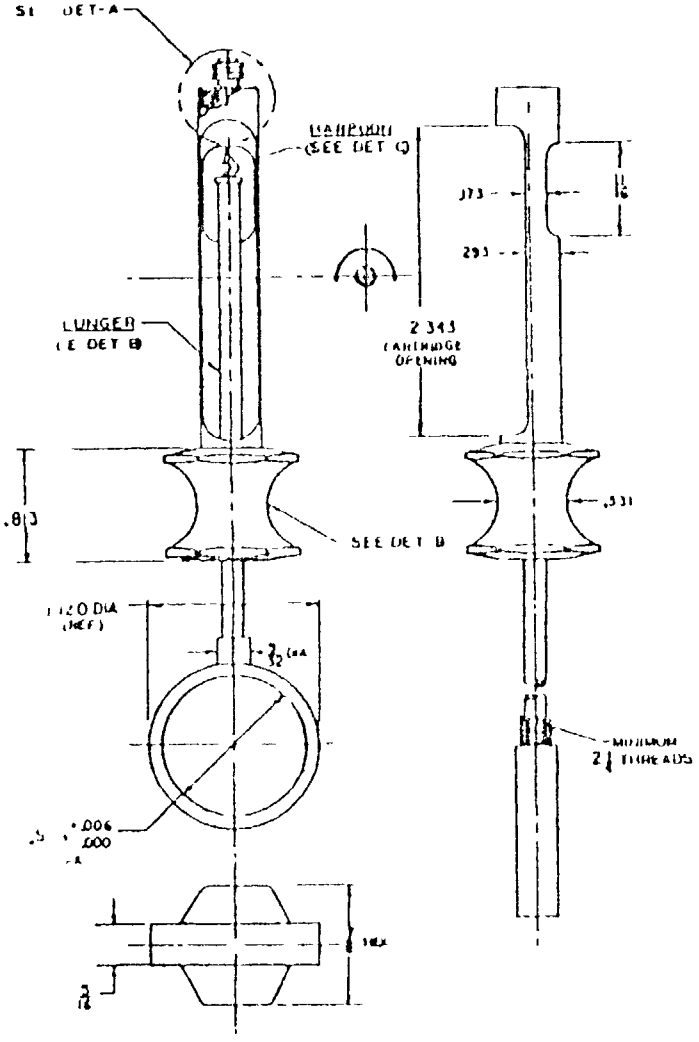

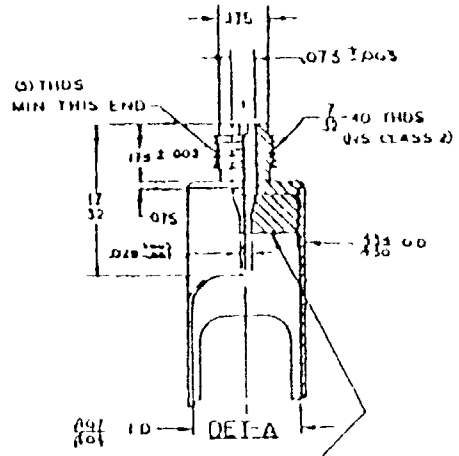

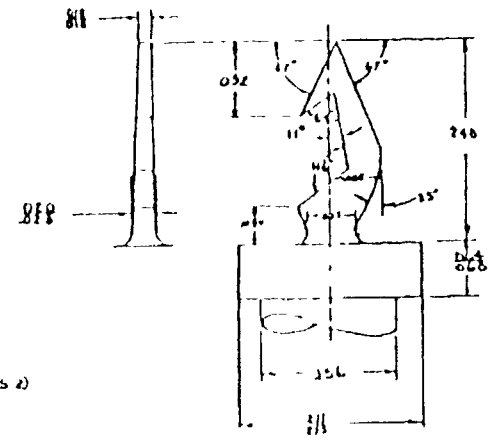

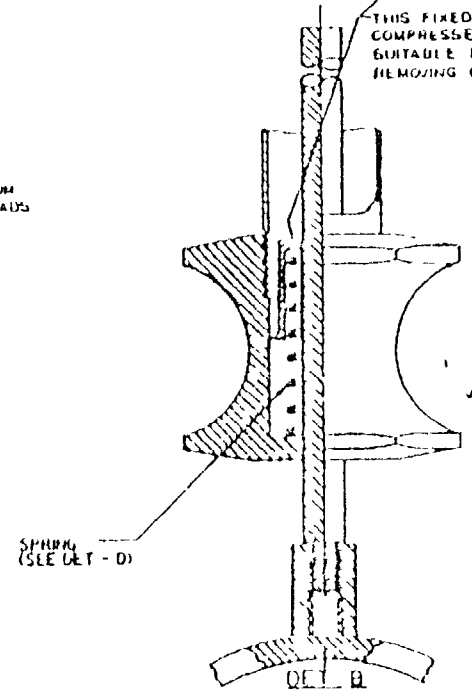

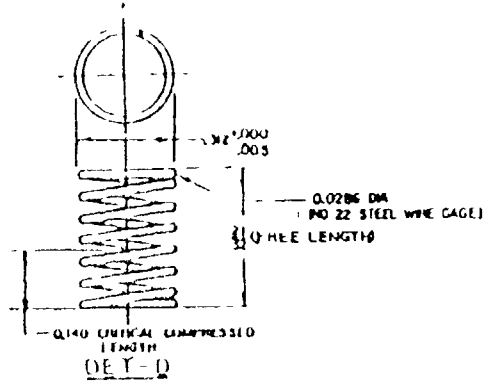

NSN 6515-01-010-8761

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES. TOLERANCES ON:		
FRACTIONS	DECIMALS	ANGLES
± 1/64	± 005	± °

FIGURE 1 ...IGE, CARTRIDGE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 [illegible] and 5 blank with the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7.

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER 2-A-54922	2 DOCUMENT DATE (YYMMDD) 931008

3 DOCUMENT TITLE
SYRINGE, CARTRIDGE, ASPIRATING

4 NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed.*)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	e DATE SUBMITTED (YYMMDD)

7 PREPARING ACTIVITY

a NAME Defense Personnel Support Center ATTN: DPSC-MSE	b TELEPHONE (Include Area Code) (1) Commercial: (215)7372870 (2) AUTOVON: 444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756 2340 AUTOVON 289-2340

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.