INCH-POUND

A-A-54924
8 October 1993

COMMERCIAL ITEM DESCRIPTION

ADAPTERS, ENDOTRACHEAL ANESTHESIA SET

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-A-36665, which is cancelled.

This Commercial Item Description covers requirements for adapters suitable for use with standard endotracheal anesthesia circuits.

Salient characteristics:

Scope. This document covers the following types of adapters.

Type I - Right Angle Elbow
Type II - Catheter "Y"

Material. Adapters shall be fabricated from neoprene capable of withstanding repeated steam sterilization without deformation. Material shall not permanently deform or be adversely acted upon with medicinal gases generally used in anesthetic procedures.

Inserts for Type II adapters shall be fabricated from unplated martensitic or austenitic corrosion resisting steel.

Style, design and dimensions. Type I adapter shall be a right angle elbow adapter suitable for use with oronasal masks, and between 15 mm endotracheal tube connectors and Y-piece adapters when used with standard anesthesia apparatus.

Type II adapter shall be a Y-piece, catheter "Y" suitable for use between right angle elbow adapter or a 15 mm endotracheal tube connector and an inhaler tube of a standard anesthesia apparatus. This type adapter shall have an integral corrosion-resistant unplated metal insert at the patient end.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Style and dimensions of the adapters shall in accordance with Figure 1.

Performance.

Sterilization. Both Type I and Type II adapters, when subjected to the following test, shall show no indication of damage, separation, deformation, or corrosion of the metal insert.

The adapters shall be steam sterilized at temperature of 250°F for a period of 10 minutes or 272°F for a period of 3 minutes. The adapters then shall be removed from the sterilizer and allowed to cool to room temperature. The test shall be performed a total of 10 times.

Accelerated aging. When subjected to a temperature of 158°F ± 2°F for seven days in an air oven, neoprene material shall not become tacky or brittle.

Identification markings. Adapters shall be permanently and legibly marked with the name and registered trademark of the contractor.

Workmanship. The adapters shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One adapter of the type specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one adapter as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one adapter. Inspection level shall be S-1, acceptance number shall be zero for all sample sizes.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers and their respective Item Identifications is covered by this document:

National Stock Number	Type	Item Identification
6515-00-880-1832	I	ADAPTER, RIGHT ANGLE ELBOW, ENDOTRACHEAL ANESTHESIA SET
6515-00-880-1833	II	ADAPTER, Y-PIECE, ENDOTRACHEAL ANESTHESIA SET, CATHETER "Y"

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5509
Location: c:tarun/adapters

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

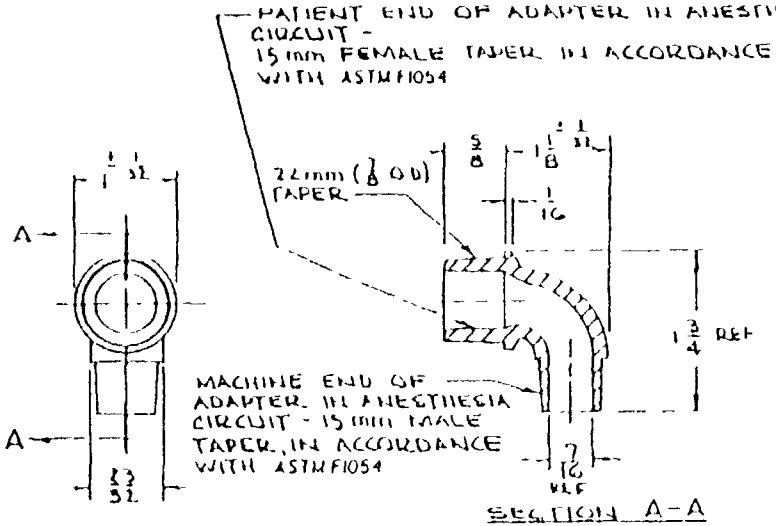

ADAPTER, RIGHT ANGLE ELBOW
TYPE I
NSN6515-00-880-1852

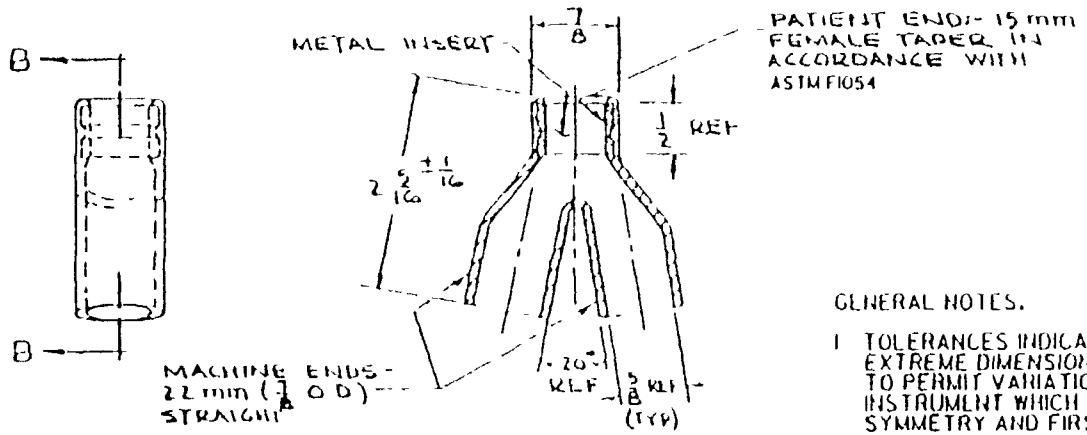

ADAPTER, Y PIECE, CATHETER "Y"
TYPE II
NSN6515-00-880-1833

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES

TOLERANCES ON:		
FRACTIONS	DECIMALS	ANGLES
±1/64	±	± °

GENERAL NOTES.

1. TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.
2. PATIENT AND MACHINE ENDS TO BE FREE FROM FLASH

FIGURE 1. ADAPTERS, PHOTOCHE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, and 3. In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7.

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54924	2 DOCUMENT DATE (YYMMDD) 931008

3 DOCUMENT TITLE
ADAPTERS, ENDOTRACHEAL ANESTHESIA SET

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
ADDRESS (Include Zip Code)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403 Falls Church VA 22041 3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 Previous editions are obsolete 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

0102 – LF – 009 – 2700