INCH-POUND
A-A-54931
10 December 1993

COMMERCIAL ITEM DESCRIPTION

RETRACTOR, RIB, Finocchieto

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers a rib retractor of the Finocchieto design suitable for retracting and retaining in position, the ribs during thoracic surgical procedures.

Salient characteristics:

General. The retractor shall be a medium rib retractor with a 10 inch spread of the Finocchieto design having two straight arms; one fixed to a rack and the other movable along the rack.

Material. The material shall be Class 4 stainless steel, as an alternate the handle and rivets shall be Class 3 stainless steel, in accordance with the American Society for Testing and Materials (ASTM) F899.

Style, design and dimensions. The retractor shall be in accordance with Figures 1 and 2 for style, design and dimensions.

Hardness. The retractor shall have a Rockwell Hardness C scale (HRC) of 40 to 48 for Class 4 stainless steel and an HRB of 75 to 95 for Class 3 stainless steel when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Finish. The finish of the retractor shall be satin.

Passivation. The retractor shall be properly passivated.

Corrosion resistance. The retractor shall show no signs of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM Designation F1089.

Identification marking and labeling. The retractor shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Retractors of foreign manufacture shall bear the name of the country of origin.

Performance. Assemble the movable arm, handle and pinion to the rack then rotate the handle several times to ensure that the pinion and rack teeth engage correctly.

Workmanship. The retractor shall be uniform and free from cracks, pits, burrs, sharp edges, scale, rough areas, corrosion, grind or tool marks, and dirt or polishing materials.

Unit. Each (EA). One retractor as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one retractor. Sampling shall be Inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one retractor. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-00-361-7250	RETRACTOR, RIB, Finocchieto

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

FDA-MPQAS
USPHS
VA-OSS

Project No: 6515-5653
Location: Intergraph/rib

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

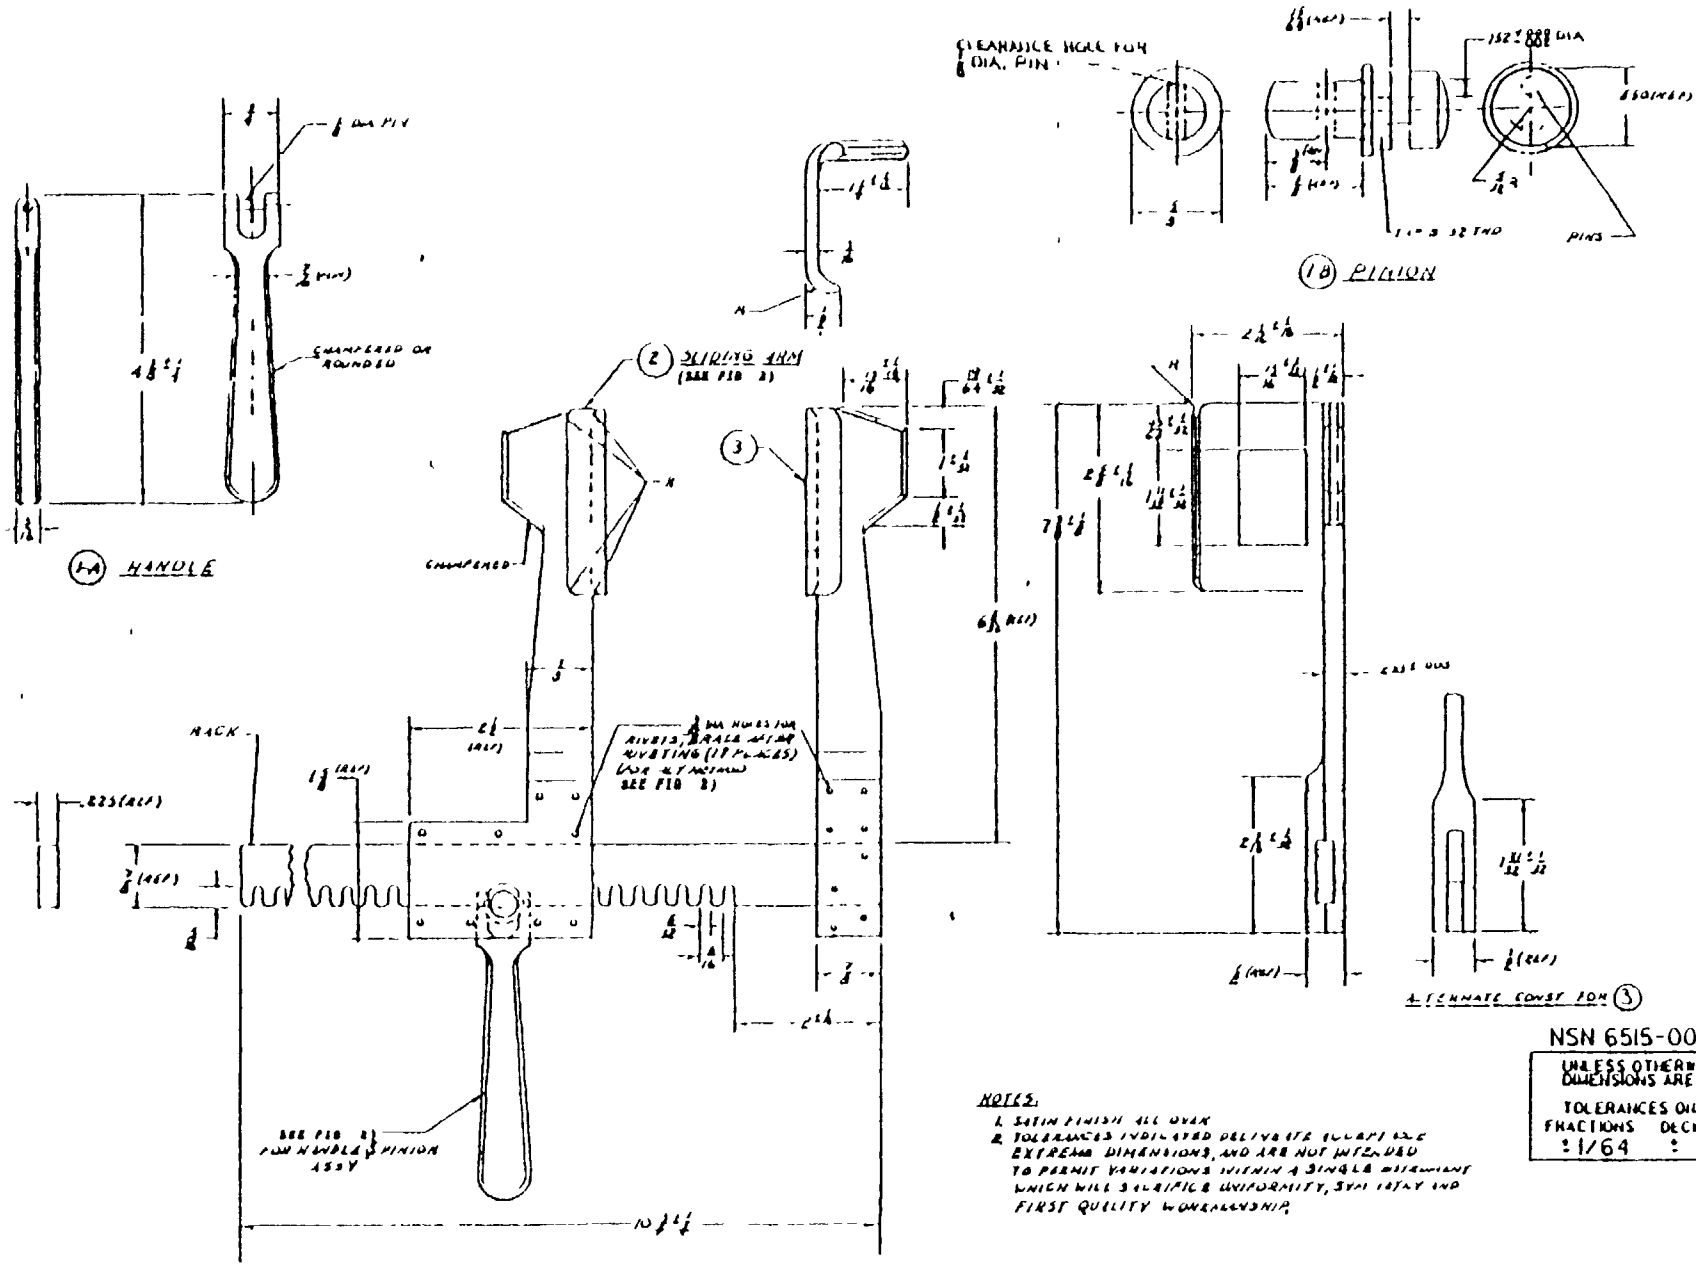

NSN 6515-00-361-7250


UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
±1/64	±	±


4-4- 54931

FIGURE 1 RETRACTOR, RIB, [illegible] CHIEF

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.


A-A-54931

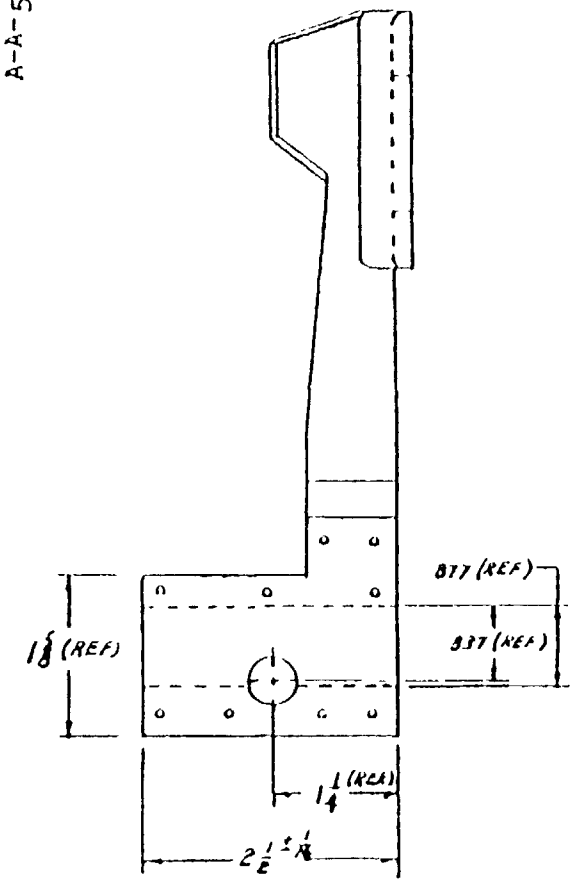

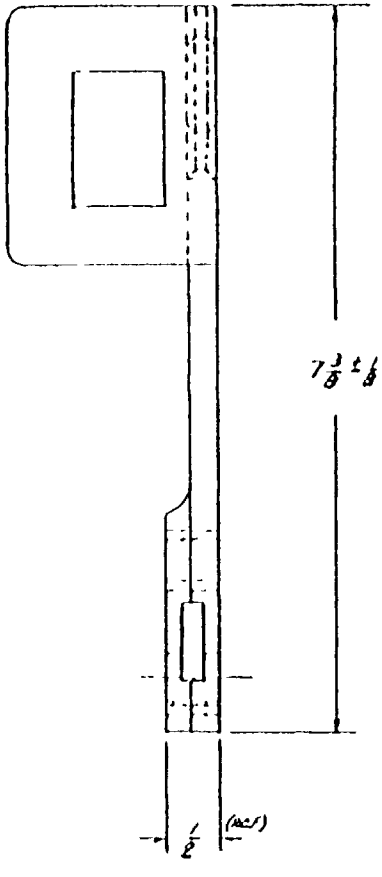

(2) SLIDING ARM

DIMENSIONS FOR PARTS 2 & 3 SIMILAR EXCEPT AS NOTED (SEE FIG 1)

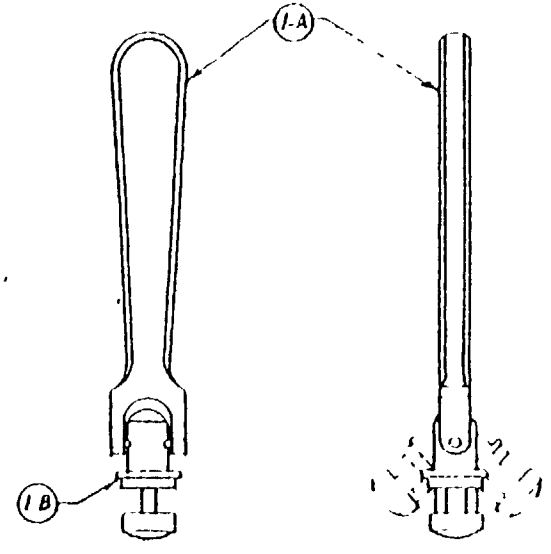


(1) HANDLE ASSY

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES

TOLERANCES ON:

FRACTIONS	DECIMALS	ANGLES
± 1/64	±	± °

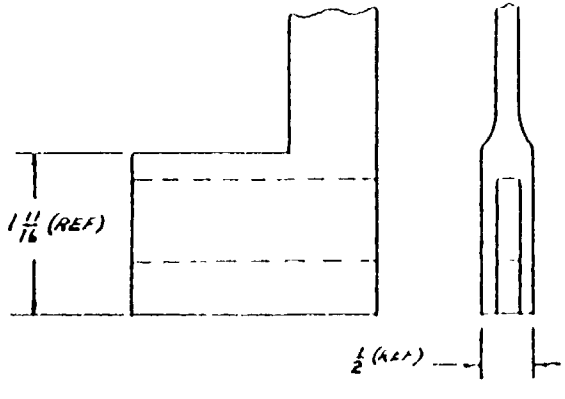

ALTERNATE CONSTRUCTION FOR SLIDING ARM

FIGURE 2 RETRACTOR RIB, FINOCCHIETO

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-54931	931210

3 DOCUMENT TITLE

RETRACTOR, RIB, Finocchieto

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed.)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215) 7372870	444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.