INCH-POUND

A-A-54940
31 January 1994

COMMERCIAL ITEM DESCRIPTION

NEEDLE, HYPODERMIC, BLOOD COLLECTING

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Interim for Federal Specification GG-N-00195B (DSA-DM), which is cancelled.

This Commercial Item Description covers sterile disposable double pointed hypodermic blood collecting needles.

Salient characteristics:

Classification.

Type I - without shut-off sleeve
Type II - multiple sample with shut-off sleeve

Material. The needle cannula shall be fabricated from Class 3, Type 304 stainless steel in accordance with American Society for Testing and Materiel (ASTM) F899. The hub shall be fabricated from rigid polypropylene that meets the United States Pharmacopeia (USP) requirements for Class IV plastics. The shut-off sleeve of the needle shall be fabricated from latex rubber or natural rubber which meets the USP requirements of Elastomeric Closures For Injections. The holder shall be fabricated from translucent medical grade polypropylene. The protective sheaths shall be fabricated from rigid plastic.

Style and design. Shall consist of a thin wall 20 gauge double pointed needle with protective sheath on each end. The needle shall have a threaded hub designed to attach to the tube holder. The tube end of the needle shall be open at the proximal end and shall be covered by a rubber shut-off sleeve which shall be securely attached to the hub (Type II only). The shut-off sleeve shall operate automatically as the blood collecting tube is forced against the needle displacing the shut-off sleeve. Withdrawal of the blood collecting tube shall result in resealing the blood

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

collecting needle. The needle shall be 20 gauge by 1-1/2 ± 1/16 inches long on the patient end with the following dimensions (inches):

Overall length	Cannula ID	Point length
2-9/16 ± 1/8	0.035 ± 0.001	0.148 - 0.180

The hub shall have the following dimensions (inches):

Hub Diameter	0.280 ± 0.002
Hub Thread, Double	0.185 - 18 NS
Major Diameter	0.185 + 0.010 - 0.005
Minor Diameter	0.139 + 0 - 0.004
Pitch Diameter	0.164 + 0 - 0.004

The blood collecting tube holder shall be designed for use with evacuated blood collecting tubes and double-pointed blood collecting needles.

One end of the holder shall be entirely open for the free insertion of a vacuum blood collecting tube. The open end shall have a flange around its periphery suitable for an ample finger hold. Opposite segments of the flange shall be shaped so as to check rolling. The opposite end of the tube shall be closed except for a centrally located passage, threaded so as to form a secure fit with double-pointed, blood collecting needles. A permanent guideline perpendicular to the vertical axis of holder shall be located 7/32 inch from the inside bottom on the threaded end. The guideline shall be situated so that after the needle is screwed into the holder and the tube is inserted so that the top of the stopper meets the guideline, the rear point of the needle shall be embedded in the diaphragm and shall not puncture it.

Dimensions of the holder in inches shall be as follows:

Overall length	2.10 ± 0.01
ID(max.)	0.720 (open end)
ID(min.)	0.700 (needle end)
Female thread, double	0.193 - 16NS
Major diameter	0.193 + 0 - 0.002
Pitch diameter	0.175 + 0 - 0.003
Minor diameter	0.150 + 0.003 - 0

The style and design shall be in accordance with Figure 1.

Non-toxic and pyrogen-free. The needle shall be non-toxic and pyrogen free when tested in accordance with USP.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Sterility. The needle shall be tested for sterility in accordance with USP or AAMI requirements. Sterility assurance level shall be 0.0001.

Resistance to separation. The needle cannula shall not separate from the hub when subjected to a 5 pound axial tensile force exerted for one minute (See note 3).

Workmanship. The needle shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing 1000 individually packaged sterile hypodermic needles of one type only, together with 10 blood collecting tube holders, as specified, constitutes one unit. As an alternate, ten boxes containing 100 individually packaged needles each, together with a suitable box or bag containing the holders, may be supplied. Each needle shall be packaged in a suitable sealed container capable of maintaining sterility of contents unless package is damaged or opened. Cannula used to enter the vein shall be protected by a sheath in such a manner that by turning the sheath the hub shall be screwed into the orifice of the tube holder without the use of instruments.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:40Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one blood collecting hypodermic needle and one holder as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one blood collecting hypodermic needle and one holder. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

NOTE 1: The following National Stock Numbers and thier respective Item Identifications is covered by this document:

National Stock Number	Item Identification
6515-01-003-2368	NEEDLE, HYPODERMIC, Blood Collecting, Multiple Sample, Double Pointed, 20 gauge, 1000s
6515-01-003-2369	NEEDLE, HYPODERMIC, Blood Collecting, Double Pointed, 20 gauge, 1000s

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

NOTE 2: As alternate test, such as a pull-to-destruction test is acceptable in lieu of the 5 pound separation test, provided product found acceptable of the pull-to-destruction test also passes the 5 pound separation test.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5606
Location: c:mark/blood3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

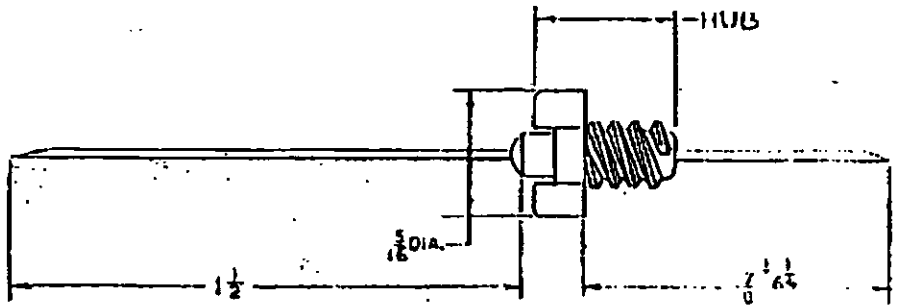

NEEDLE, W/O SHEATH

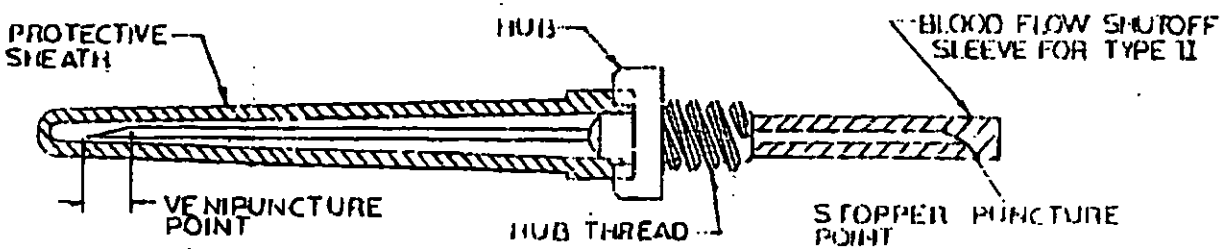

NSN 6515-01-003-2368

NEEDLE, WITH SHEATH

NOTE:
1. DIMENSIONS ARE IN INCHES.
2. DESIGN VARIATIONS ALLOWED PROVIDED NEEDLE DOES NOT DEVIATE FROM OTHER REQUIREMENTS OF THE SPECIFICATION.

FIGURE I - NEEDLE, TYPE I AND TYPE II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.