INCH-POUND

A-A-54941
31 January 1994

COMMERCIAL ITEM DESCRIPTION

CHISEL, PERIODONTAL
(Double-ended)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-C-42003(DM), which is cancelled.

This Commercial Item Description covers a double-ended chisel for use in periodontal surgical and scaling procedures.

Salient characteristics:

Material. Stainless steel shall be in accordance with American Society for Testing Material (ASTM) Designation F899 and brass shall conform to Class 8, copper alloy number 330, as specified in ASTM Designation B135 for composition only.

Operative ends. The operative ends shall be Class 4, martensitic stainless steel, Type 440A, B or C.

Handle. The handle shall be fabricated of chromium over nickel plated brass, Class 3, austenitic, Class 4, martensitic or Class 6, ferritic, Type 430F stainless steel.

Hardness. After proper stress relieving, the Rockwell hardness of the operative ends shall be C52 to C57 for Type 440A, C52 to C58 for Type 440B, and C56 to C60 for Type 440C. Handles and shanks shall be of proper temper and shall have a hardness suitable for the purpose intended. Hardness shall be determined in accordance with ASTM Designation E18 (Rockwell) or E92 (Vickers or Diamond Pyramid).

Design and dimensions. Shall be a double-ended Kirkland 13K and 13KL pull chisel suitable for use in periodontal osseous surgery and as a heavy scaler of teeth and exposed root surfaces. The design and dimensions of the chisel operative ends and shank shall conform to Figure 1. The chisel shall be furnished with the handle design as shown in Figure 2.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

Construction. The chisel shall be of a three piece construction consisting of a handle and an operative end at each end. The handle shall be solid or hollow and have a round or octagonal cross section. Knurled of serrated portions of handles shall be as specified in Figure 1. The operative ends shall be permanently secured to the handle. Junction of operative end to handle shall be smoothly finished and free of crevices. There shall be no movement, loosening, or separation between the operative end and handle when the operative end is subjected to an 85 pound (minimum) pull out force, when tested as specified.

Finish. The operative ends, including shanks, shall have a smooth mirror or smooth bright finish, except for sharpened edges which shall have a finely honed finish. The operative ends shall have a sharp cutting edge and shall be free of defects, such as coarse grind marks, cracks, gouges, burrs, feathers, or other imperfections which affect performance. Finger grip portions of handles shall be serrated or knurled. Handles shall have a mirror or bright finish, except for the serrated or knurled portions. Finger grip portions of handles shall be free from barbs and shall provide adequate finger grip during use.

Corrosion resistance. The copper sulfate test requirements of ASTM Designation F1089 shall apply to the operative ends, martensitic and ferritic stainless steel handles. The boil test requirements of ASTM Designation F1089 shall apply to the entire chisel (operative ends and all handles).

Identification markings. Each chisel shall be marked with the respective Kirkland instrument numbers, as applicable. All markings shall be on the smooth portion of the handle. Each chisel shall be marked with the name or registered trademark of the manufacturer (and contractor, if other than the manufacturer). The word "stainless", when applicable, shall also be marked on instruments of foreign manufacture. As an alternate to the word "stainless", the use of a registered trade name identifying the steel as stainless shall be acceptable, provided prior approval is received from the cognizant contracting officer.

Workmanship. The operative end shall be free of rounded edges. The entire instrument shall be free of deep pits, discoloration and other defects which may detract from their appearance or impair their intended use.

Unit. Each. (EA). One chisel, as specified, constitutes one unit. Each chisel shall be packaged in a suitable

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

sealed container. As an alternative, each chisel shall be supplied in a rigid plastic tube with a metal screw cap or a plastic friction plug closure; cushioning shall be used to prevent damage to the operative ends.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for examination purposes shall be one chisel. Sampling shall be inspection level S-2. Acceptance level shall be zero for all sample sizes.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one chisel. Sampling shall be

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

inspection level S-2 with an AQL (Acceptable Quality Level) of 1.0.

Pull test. The handle and shank of the operative end shall be securely held in separate chucks or other holding devices. A slowly increasing pull out force, increasing from zero to 85 pounds (minimum), shall be applied to the shank of the operative end. The force shall be maintained at the high value for a minimum of 1 second. The instrument shall then be examined for movement, looseness, or separation of the operative end with respect to the handle. The test shall be repeated for each operative end of the double-ended instrument.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements

of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

NOTE: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6520-01-093-2280	CHISEL AND SCALER, PERIODONTAL, Kirkland No. 13K and 13KL

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6520-2536
Location: word\doc\preston\chisel

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

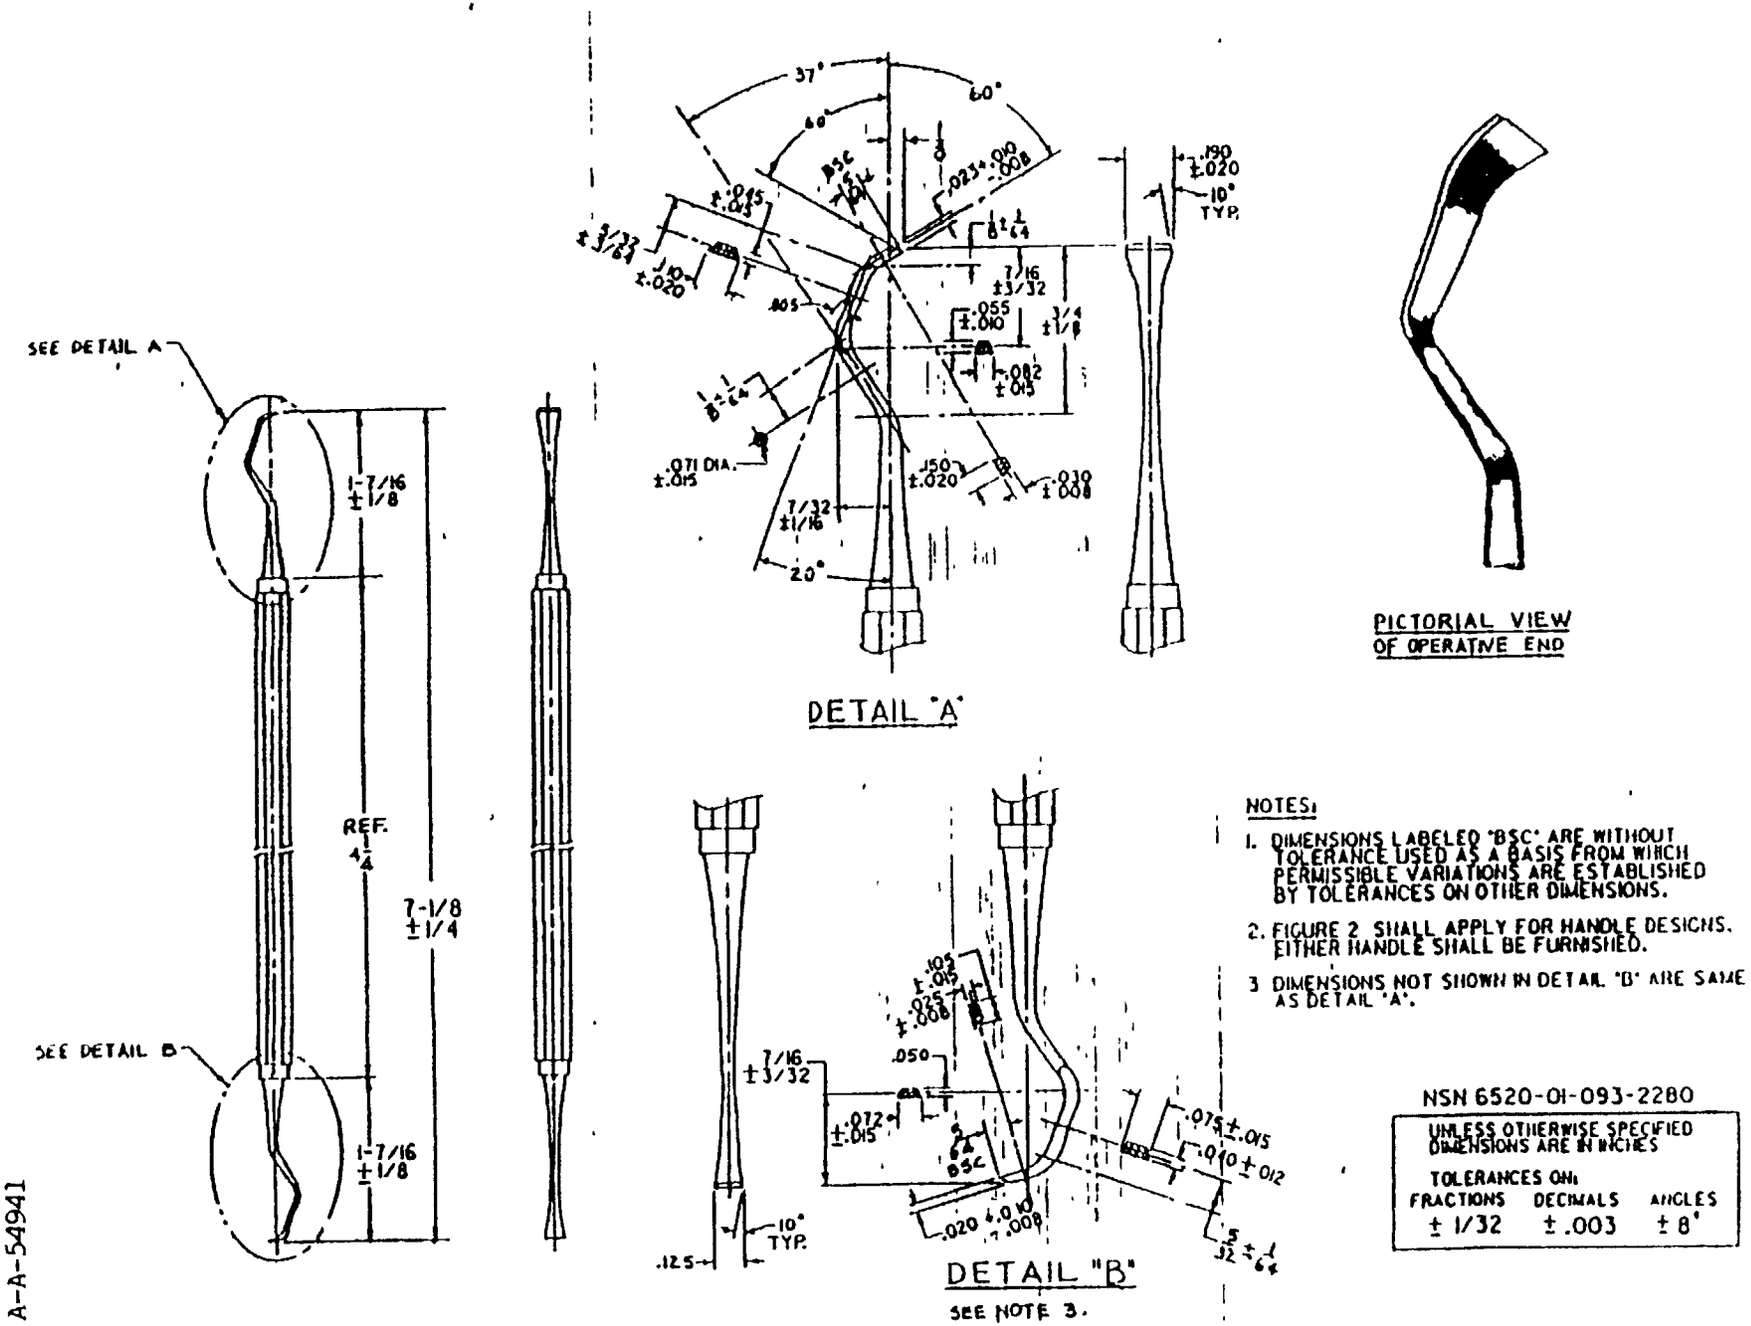

NOTES:

1. DIMENSIONS LABELED "BSC" ARE WITHOUT TOLERANCE USED AS A BASIS FROM WHICH PERMISSIBLE VARIATIONS ARE ESTABLISHED BY TOLERANCES ON OTHER DIMENSIONS.
2. FIGURE 2 SHALL APPLY FOR HANDLE DESIGNS. EITHER HANDLE SHALL BE FURNISHED.
3. DIMENSIONS NOT SHOWN IN DETAIL "B" ARE SAME AS DETAIL "A".


NSN 6520-01-093-2280

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON:		
FRACTIONS	DECIMALS	ANGLES
± 1/32	± .003	± 8°


A-A-54941

FIGURE 1. CHISEL AND SCALER, PERIODONTAL, KIRKLAND NO. 13K AND 13KL, DOUBLE-ENDED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

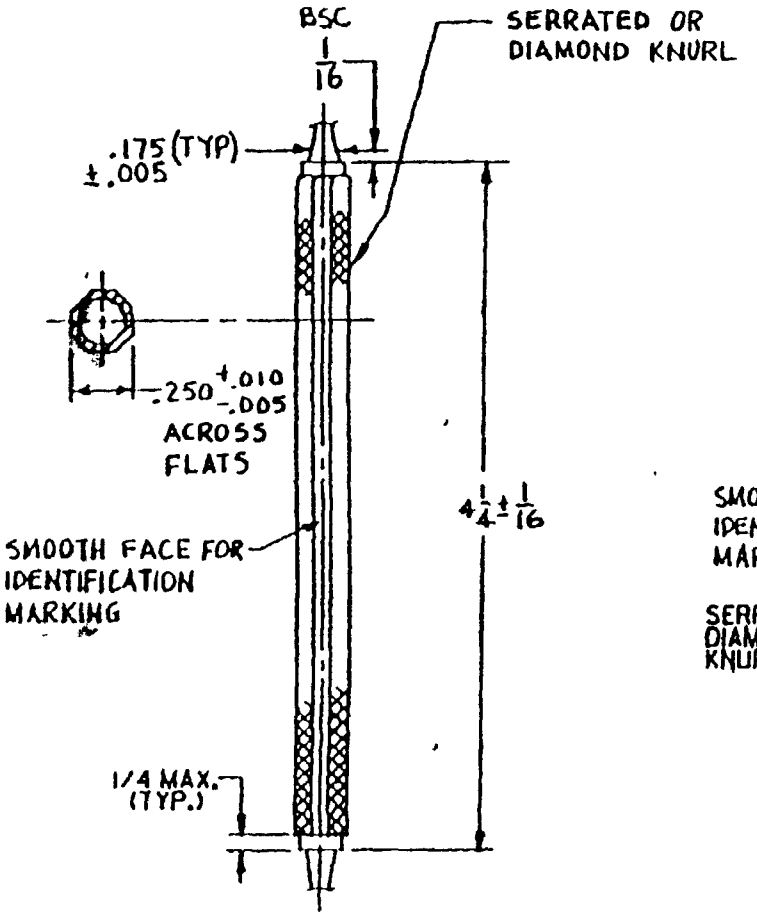

OCTAGONAL HANDLE

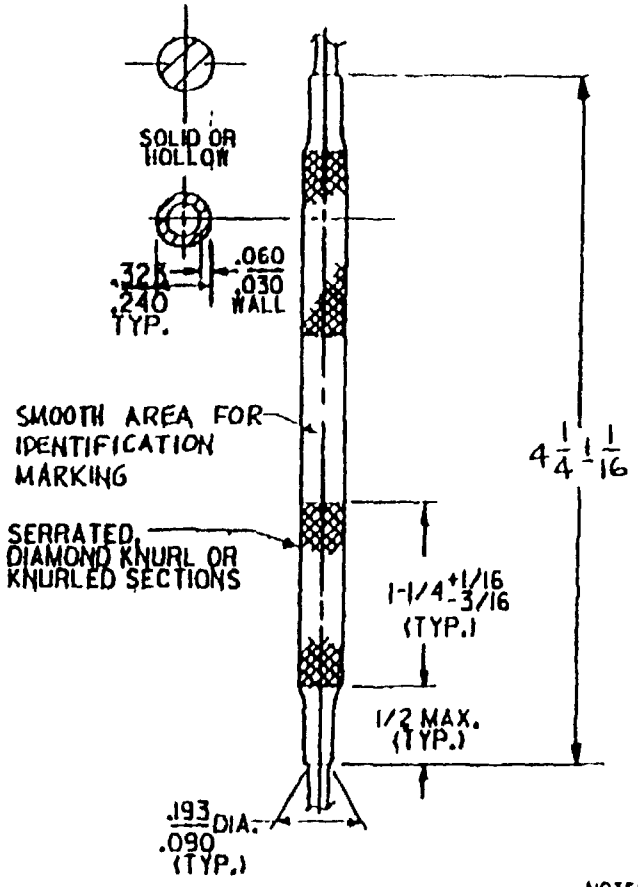

ROUND HANDLE

NOTES:

1. DIMENSIONS LABELED "BSC" ARE BASIC WITHOUT TOLERANCE USED AS A BASIS FROM WHICH PERMISSIBLE VARIATIONS ARE ESTABLISHED BY TOLERANCES ON OTHER DIMENSIONS.
2. HANDLES SHALL BE IN ACCORDANCE WITH THIS DRAWING FOR DIMENSIONAL REQUIREMENTS. SHAPE OF HANDLES SHOWN ARE TYPICAL, AND ARE NOT INTENDED TO RESTRICT OR PRECLUDE THE PURCHASE OF INSTRUMENTS WHICH ARE OTHERWISE IN ACCORDANCE WITH THIS SPECIFICATION.
3. ALL DIMENSIONS IN INCHES UNLESS OTHERWISE SPECIFIED.

FIGURE 2 HANDLES, DENTAL, PERIODONTAL INSTRUMENTS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	A-A-54941	940131

3. DOCUMENT TITLE
CHISEL, PERIODONTAL (Double-ended)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)
	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial: (215)7372870 (2) AUTOVON: 444-2870
ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:40Z
Check the source to verify that this is the current version before use.