MIL-C-2592A
6 June 1967
SUPERSEDING MIL-C-2592
7 February 1951, Army 10-2575
27 April 1939 and MIL-H-36324
(DM) 3 November 1964

MILITARY SPECIFICATION

CAUTERY, HANDLE

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers three types of cautery handles.

1.2 Classification. Cautery Handles covered by this specification shall be of the following types:

Type 1. Pencil.
Type 2. Pistol Grip.
Type 3. Straight.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper, (for Carton Sealing).

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer).

3. REQUIREMENTS

3.1 First Article. Unless otherwise specified, prior to the start of production of the contract quantity, one sample handle of each type shall be assembled, completely finished, and tested by the contractor. The sample(s) shall be submitted, together with the contractor's inspection and test reports, to the procuring contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the procuring contracting officer, or his authorized representative, prior to the manufacture and assembly of the remaining quantity to be manufactured. Pending approval of the first article(s), acquisition of materials, components, or commencement of production is at the sole risk of the contractor. Accepted sample shall become the property of the procuring activity and shall be included in the quantity called for in the contract or order. In the event that the sample is not approved, the contractor shall submit a new sample for approval, or modify the existent sample so as to remove the deficiencies cited.

3.2 Material. Material shall be of high quality and suitable in all respects for the purpose intended. The metal conductors shall be of sufficient current capacity to carry the necessary operating current without undue resistance or heating. The body of the unit shall be fabricated from a non-conducting, sturdy plastic. Metal shall be of a high grade quality, best suited for this type of instrument, uniformly chromium or nickel plated and highly polished. Contact points shall be platinum.

3.3 Construction. The cautery handles shall be as indicated herein for appropriate type. The dimensions cited shall not vary from the nominal dimensions indicated by more than plus or minus 10 percent.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

3.3.1 Type 1 Handle "Cautery Pencil". The type 1, Handle Cautery Pencil, (see figure 1) shall be an optical and nasal cautery handle, pencil type. A sensitive button switch shall be located near the operative end. A 5-foot minimum electrical cord complete with a male attachment on distal end shall be attached to the handle. The female shank socket shall be constructed and spaced to accept cautery tip shanks of 1/16-inch diameter by 11/32-inch long, spaced on 9/64-inch centers. The handle shall be circular in cross section, 3/8-inch in diameter and 3-1/2-inch in length. Two metal stems, insulated from each other, shall be incorporated within handle longitudinally. Stems shall protrude from distal end of handle nominally 1/8-inch and 1 1/4 inches from proximal end. The distal protruding ends shall have female fittings for friction fitting of prongs on cautery electrodes. These openings shall accept prongs 9/16-inch in length, 0.045 inch in diameter. There shall be 3/32-inch distance between prongs. The proximal ends of the stems shall be fitted with female fittings incorporating set screws, for acceptance of cord tips. Openings in fittings shall be 13/16-inch in depth and 1/16-inch in diameter. The contact breaker or switch shall be incorporated inside of handle and shall be operated by a conveniently located, plastic, removable button plunger.

3.3.2 Type 2 Handle, Cautery, Pistol Grip. The type 2, Handle, Cautery Pistol Grip, (see figure 2) shall be provided with a 5 foot minimum electrical cord, equipped with 1/8 by 3/4-inch pin jacks with insulated finger grips, one for each wire. The handle shall be equipped with female sockets suitable to accept cautery electrodes having double shanks with the following dimensions:

Shank diameter inch	Shank spacing, center to center-inch	Length-inch
0.1055 (No. 12 Washburn and Moen)	0.300	1-1/2
0.0915 (No. 13 Washburn and Moen)	0.347	1-7/16

The dimensions of the handle shall be 3-3/4 to 5 inches long, 1-3/16 to 1-15/16-inches wide, and 2-1/2 to 2-7/8 inches at the top of the handle where the set screw is attached. A switch button for momentary or continuous operation shall be mounted in a convenient place. The handle shall be suitable for use with electrodes requiring an operating current of up to 40 amperes, and a voltage of 1.5 to 2.0 volts.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

3.3.3 Type 3 Handle,Cautery, Straight. The type 3 Handle Cautery Straight, (see figure 3), shall be rectangular in cross section, surrounding two metal stems which run thru it lengthwise and project at both ends of the handle. The handle, excluding fittings, shall be four inches long, 3/4-inch wide and 3/8-inch thick. Distal fittings projecting 1/2-inch from handle, shall have two female set screw fittings to accept the items of the cautery electrodes. The openings in the female fittings shall be so arranged that the cautery electrode is capable of being mounted, either in the axis of the handle, or to form an angle of 115 degrees with the handle. Openings shall be 3/32-inch in diameter, and shall be 3/8-inch apart between centers. Proximal end of stems shall project nominally 1-5/16-inch from handle and shall have set screw female openings to accept tips of cautery cord. Each of these openings shall be 7/16-inch in depth and 3/32 inch in diameter. The switch shall be incorporated inside of handle and shall be operated by a conveniently located plastic button plunger. The button plunger shall be located on the distal end of handle opposite cautery when the latter is attached at the angle specified.

3.4 Identification marking. Each handle shall be permanently and legibly marked with contractors name or registered trade-mark.

3.5 Workmanship. Workmanship shall be first class throughout. Handles shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Supplier responsibilities for inspection. Such examinations and tests as are set forth in this specification or as shall otherwise be appropriate or necessary to insure that the supplies conform to specification requirements, shall be performed by and at the expense of the supplier. Suppliers who do not have facilities adequate for such tests shall arrange for the use of test facilities acceptable to the Government. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government, upon the Government's request, at any time, or from time to time, for a period of 2 years after delivery of the supplies to which such records relate.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory,investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with Military Standard MIL-STD-105.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with Military Standard MIL-STD-105.

Component (unit of product)	Characteristic	Requirement	Test procedure	Rqmt. Appl. Indiv unit	Rqmt. Appl. Lot avg	Sample unit	Inspection level	AQL
(end item)	Dimensions	3.3.1 3.3.2 3.3.3	4.3	1 handle			S2	4.0

* A minimum of three units shall be tested regardless of lot size.

4.3 Examination. The handles shall be examined to determine compliance with applicable requirements contained in this specification.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One handle, as specified, constitutes one unit if issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Type	Unit package	Intermediate package	Exterior container
1	1 unit	6	72 units
2	1 unit	Not required	48 units
3	1 unit	6	288 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive materials.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1A-15.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes, shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with appendix of applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).
(c) When first article is not required (see 3.1)
(d) When first article shall be sent (see 3.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Category N.

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

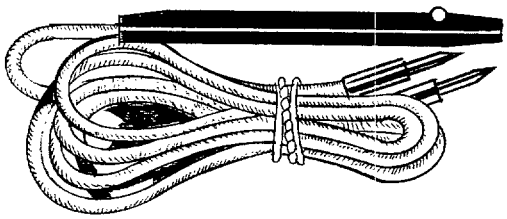


FIGURE 1 CAUTERY HANDLE, PENCIL FSN 6515-318-5800

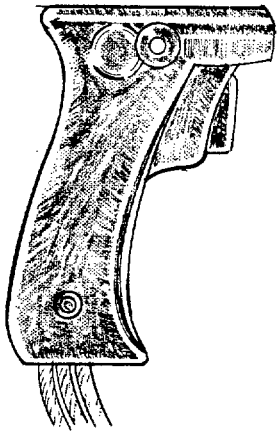


FIGURE 2 CAUTERY HANDLE, PISTOL GRIP FSN 6515-318-5900



FIGURE 3 CAUTERY HANDLE, STRAIGHT FSN 6515-318-6100

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

MIL-C-2592A

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426

REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-16T15:09Z
Check the source to verify that this is the current version before use.