PERFORMANCE SPECIFICATION SHEET

METERS, ELECTRICAL INDICATING, PANEL TYPE, RUGGEDIZED: VOLTMETER, DC (FLUSH MOUNTING, ROUND FLANGE, 3½ INCH), STYLE 36

This specification is approved for use by all Departments and Agencies of the Department of Defense.

The requirements for acquiring the meters described herein shall consist of this specification and MIL-PRF-10304.

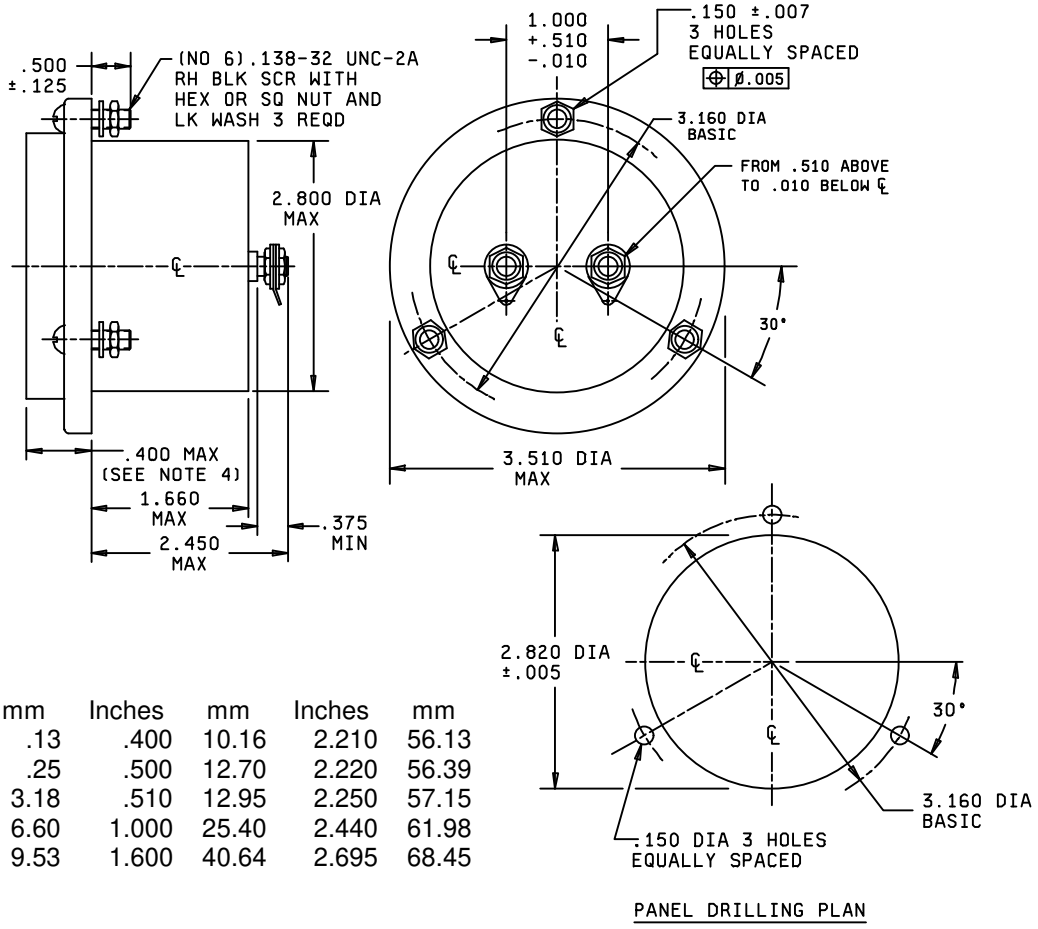

PANEL DRILLING PLAN

Inches	mm	Inches	mm	Inches	mm
.005	.13	.400	10.16	2.210	56.13
.010	.25	.500	12.70	2.220	56.39
.125	3.18	.510	12.95	2.250	57.15
.260	6.60	1.000	25.40	2.440	61.98
.375	9.53	1.600	40.64	2.695	68.45

NOTES:
1. Dimensions are in inches.
2. Metric equivalents are given for general information only.
3. Tolerance is ±1/2° on angles.
4. Maximum projection from front panel including mounting gaskets (if used).

FIGURE 1. Meter, panel type.

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T13:48Z
Check the source to verify that this is the current version before use.

REQUIREMENTS:
(Readings expressed as a percent of full-scale value.)

Dimensions and configuration: See figure 1.

Full-scale ranges: See table I.

Scale:
Length: 2 inches minimum.
Pointer deflection: 90° minimum.

Position influence: ±2 percent change of 60° rotation from normal operating position.

Accuracy: ±2 percent.

Overshoot: 50 percent maximum.

Response time: 2 seconds maximum.

Power consumption (loss) (at end scale deflection): 1 mA ±5 percent.

High temperature cycling:
±3 percent.
±2 percent permanent change.

Temperature influence: ±0.75 percent change.

Exposure to extreme temperatures: ±3 percent permanent change.

Overload capacity:
±1 percent temporary zero shift.
±1 percent permanent zero shift.
±2 percent permanent change.

Dielectric withstanding voltage: 3,000 volts rms.

TABLE I. Full-scale ranges.

Volts				Kilovolts 1/	
Zero left		Zero center			
2 10	20 30 50 100	150 200 300 500 800	30-0-30 50-0-50 100-0-100 200-0-200	1 2 5	10 20 30

1/ Used with external resistor. These meters shall have a full-scale deflection of 1 milliampere, with 150 millivolts terminal drop. Requirements for these meters shall be as specified for milliameters in accordance with MIL-PRF-10304/12.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T13:48Z
Check the source to verify that this is the current version before use.

Custodians:
Army - CR
Navy - SH
Air Force - 99
DLA - CC

Review activities:
Army - AR, AT, AV, CR4

Preparing activity:
DLA - CC

(Project 6625-0867)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T13:48Z
Check the source to verify that this is the current version before use.