
MIL-M-10304/9B
27 April 1971
SUPERSEDING
MIL-M-10304/9A
14 June 1965

MILITARY SPECIFICATION SHEET


METERS, ELECTRICAL INDICATING, PANEL TYPE, RUGGEDIZED: SPECIAL (FLUSH MOUNTING, ROUND FLANGE, 2-1/2 INCH) STYLE 26

The complete requirements for procuring the meters described herein shall consist of this document and the latest issue of Specification MIL-M-10304.

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

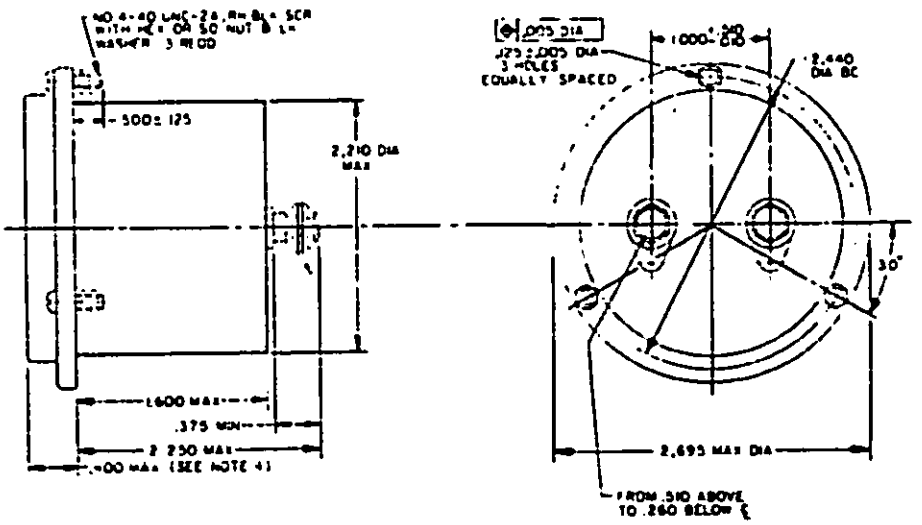

INCHES	MM	INCHES	MM	INCHES	MM
.005	.13	.400	10.16	2.210	56.13
.010	.25	.500	12.70	2.220	56.39
.125	3.18	.510	12.95	2.250	57.15
.260	6.60	1.000	25.40	2.440	61.98
.375	9.53	1.600	40.64	2.695	68.45

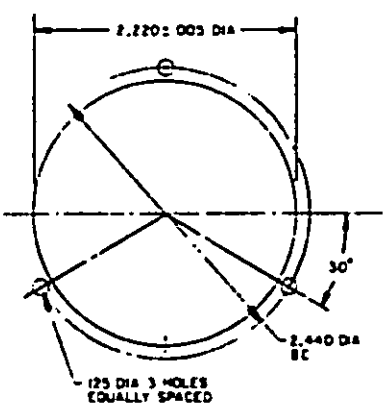

PANEL DRILLING PLAN

NOTES:
1. Dimensions are in inches.
2. Metric equivalents (to the nearest .01 mm) are given for general information only and are based upon 1 inch = 25.4 mm.
3. Tolerance is ± 1/2° on angles.
4. Maximum projection from front of panel including mounting gaskets (if used).

(B) denotes changes

FSC 6625

Source: https://assist.dla.mil -- Downloaded: 202610-17T13:47Z
Check the source to verify that this is the current version before use.

REQUIREMENTS:
(See tables I and II):

Dimensions and configuration: See figure and table II.

Full-scale range: See table I.

Scale:
Length: 1.5 inches minimum.
Pointer deflection: 90° minimum.

Position influence: ±2 percent change of full-scale length for 60° rotation from normal operating position.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T13:47Z
Check the source to verify that this is the current version before use.

Ⓑ TABLE I. Full-scale ranges and special features (except MR26M297SPECR).

NOTE: Special meters covered by this specification shall meet the requirements specified for similar meters, except for the following special features:

Type designation of meter 1/		Range of special meter	Special features	
Special	Similar		Resistance (nominal)	Power consumption (loss)
		direct current	ohms	millivolts ±2%
MR2**105SPECR	2/ MR26*020DCUAR	50 µA	5,000	250
MR2**106SPECR	2/ MR26*020DCUAR	100 µA	2,500	250
MR2**107SPECR	2/ MR26*020DCUAR	200 µA	1,250	250
MR2**108SPECR	2/ MR26*001DCMAR	500 µA	500	250
MR2**109SPECR	2/ MR26*001DCMAR	1 mA	100	100
MR2**110SPECR	2/ MR26*001DCMAR	1.5 mA	66-2/3	100
MR2**111SPECR	2/ MR26*001DCMAR	3 mA	33-1/3	100
MR2**112SPECR	2/ MR26*001DCMAR	5 mA	20	100
MR2**113SPECR	2/ MR26*001DCMAR	8 mA	12-1/2	100
		amperes, dc		
MR2**114SPECR	2/ MR26*010DCAAR	1-0-9	Scale marked "Charge" (to right of zero) and "Discharge" (to left of zero).	
MR2**115SPECR	2/ MR26*010DCAAR	3/ 10-0-30		
MR2**116SPECR	2/ MR26*010DCAAR	3/ 15-0-15		
MR2**117SPECR	2/ MR26*010DCAAR	4/ 25-0-75		
MR2**118SPECR	2/ MR26*010DCAAR	3/ 30-0-30		
MR2**119SPECR	2/ MR26*010DCAAR	3/ 50-0-50		
		volts, dc		
MR2**130SPECR	5/ MR26*300DCVVR	15-0-15	The range cannot be designated by the regular type designation.	
MR2**131SPECR	5/ MR26*300DCVVR	150-0-150		

			Resistance (nominal)	Power consumption (loss)	Uniform scale marking	Number of scale divisions
		direct current	ohms	millivolts ±2%		
MR2**152SPECR	2/ MR26*020DCUAR	50 µA	5,000	250	0-100	20
MR2**153SPECR	2/ MR26*020DCUAR	100 µA	2,500	250	0-100	20
MR2**154SPECR	2/ MR26*020DCUAR	200 µA	1,250	250	0-100	20
MR2**155SPECR	2/ MR26*001DCMAR	500 µA	500	250	0-100	20
MR2**156SPECR	2/ MR26*001DCMAR	1 mA	100	100	0-100	20
MR2**157SPECR	2/ MR26*001DCMAR	1.5 mA	66-2/3	100	0-100	20
MR2**158SPECR	2/ MR26*001DCMAR	3 mA	33-1/3	100	0-100	20
MR2**159SPECR	2/ MR26*001DCMAR	5 mA	20	100	0-100	20
MR2**160SPECR	2/ MR26*001DCMAR	8 mA	12-1/2	100	0-100	20
MR2**161SPECR	2/ MR26*020DCUAR	50 µA	5,000	250	0-150	30
MR2**162SPECR	2/ MR26*020DCUAR	100 µA	2,500	250	0-150	30
MR2**163SPECR	2/ MR26*020DCUAR	200 µA	1,250	250	0-150	30
MR2**164SPECR	2/ MR26*001DCMAR	500 µA	500	250	0-150	30
MR2**165SPECR	2/ MR26*001DCMAR	1 mA	100	100	0-150	30
MR2**166SPECR	2/ MR26*001DCMAR	1.5 mA	66-2/3	100	0-150	30
MR2**167SPECR	2/ MR26*001DCMAR	3 mA	33-1/3	100	0-150	30
MR2**168SPECR	2/ MR26*001DCMAR	5 mA	20	100	0-150	30
MR2**169SPECR	2/ MR26*001DCMAR	8 mA	12-1/2	100	0-150	30


1/ The asterisk is to be replaced by a letter designating the color scheme.
2/ See MIL-M-10304/5 for detail requirements.
3/ Used with external shunt.
4/ Used with 75-ampere external shunt.
5/ See MIL-M-10304/4 for detail requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-17T13:47Z
Check the source to verify that this is the current version before use.

TABLE II. Special features, meter MR26M297SPECR.

NOTE: Special meter MR26M297SPECR shall meet the requirements specified for meter MR26*020DCUAR, except for the following features:

Type designation of meter		Dial calibration								
Special	Similar	DC			Ohms		AC volts			
MR26M297SPECR	MR26*020DCUAR	Scale		µA	Scale	µA	Scale		µA
		0	0	0	∞	0	0	0	0
		2	5	12.5	1,000	8.5	2	5	4
		4	10	25	750	10	4	10	10.5
		6	15	37.5	500	15	6	15	20
		8	20	50	400	18	8	20	30.5
		10	25	62.5	300	24	10	25	42.5
		12	30	75	200	34.5	12	30	55
		14	35	87.5	180	37	14	35	69
		16	40	100	160	40.5	16	40	83
		18	45	112.5	140	45.5	18	45	97
		20	50	125	120	52	20	50	111.5
		22	55	137.5	100	60	22	55	126
		24	60	150	90	64	24	60	141
		26	65	162.5	80	69.25	26	65	155.5
		28	70	175	70	76.5	28	70	170
		30	75	187.5	60	85	30	75	184
		32	80	200	50	94	32	80	198
		34	85	212.5	45	98	34	85	211
		36	90	225	40	104	36	90	224
		38	95	237.5	35	113	38	95	237
		40	100	250	30	124	40	100	250
					28	129			
					26	134.5			
					24	140			
					22	145			
					20	150			
					18	155.5			
					16	161			
					14	169			
					12	178			
					10	187.5			
					9	193.5			
					8	199			
					7	204.5			
					6	210			
					5	215.5			
					4	221.5			
					3	228			
					2	234.5			
					1	242			
					0	250			

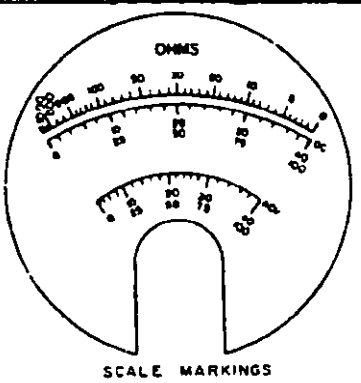

SCALE MARKINGS

Colors:
Dial . . . . . Flat white, Munsell No. N8.0
Markings, numerals, and letters:
Resistance scale. . . . Green, Munsell No. 2.5G5/8
Dc voltage and current scale. . . . . Black, Munsell No. N1.0
Ac voltage scale. . . . Purple-blue, Munsell No. 5.0PB3/12

Kind of pointer. . . . . Knife edge

Maximum projection with meter mounted on 3/8-inch panel:
In front of panel . . . . 41/64 inch
Barrel depth behind panel . . . 3/4 inch.
(A plastic spacer, if necessary to accomplish above, may be utilized and must be furnished with the meter.)

Dc range . . . . . 250 µA ±2 percent

Power consumption (loss): 62.5 mV ±2 percent at 25° ±2°C
250 ohms nominal at 25° ±2°C
270 ohms nominal at 55° ±2°C
210 ohms nominal at −40° ±2°C

Source: https://assist.dla.mil -- Downloaded: 20260-17T13:47Z
Check the source to verify that this is the current version before use.

Custodians:
Army - EL
Navy - EC
Air Force - 82

Review activities:
Army - EL, AV, AT, ME, WC
Navy - EC, MC
Air Force - 11,
DSA - ES

User activities:
Army - MI
Navy - CG
Air Force - None

Preparing activity:
Army - EL

Agent:
DSA - ES

(Project 6625-0340)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T13:47Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 202610-17T13:47Z
Check the source to verify that this is the current version before use.