MILITARY SPECIFICATION

PAD, PRE-OPERATIVE PREPARATION

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a non-sterile disposable drape suitable as an absorbent and moisture-impermeable protective bed or table cover for use under patient during pre-operating scrubbing.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-585	- Boxes, Wood, Wirebound.
PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	- Boxes, Shipping, Fiberboard.

MILITARY

MIL-L-10547	- Liners, Case, and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to : Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, Code ATT, 2800 South 20th Street, Philadelphia, PA. 19101, by using the self-addressed **Standardization Document Improvement Proposal** (DD Form 1426) appearing at the end of this document or by letter.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

STANDARDS

FEDERAL

FED-TEST METHOD STD-191	- Textile Test Methods.

MILITARY

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	- Marking for Shipment and Storage.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING & MATERIALS (ASTM)

ASTM D1117	- Standard Methods of Testing Non-Woven Fabrics.

(Application for copies should be addressed to the American Society for Testing & Materials, 1916 Race Street, Philadelphia, PA 19103.)

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)

No. 56A Standard for the Use of Inhalation Anesthetics

(Application for copies should be addressed to the National Fire Protection Association, 470 Atlantic Avenue, Boston, MA 02210.)

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

3.2 Materials.

3.2.1 Coated fabric. The coated fabric used in the construction of the pad shall consist of a white, non-woven, absorbent fabric of synthetic fibers, wood pulp, cellulosics, or any combination of synthetic fibers, wood-pulp, and cellulosics. The non-woven fabric shall be completely wetted in not more than 8 seconds when tested as specified in 4.4.1. One surface shall be coated with a suitable colored plastic, pigmented with a non-bleaching pigment. The coated fabric shall have the minimum tensile strengths listed in table I, when tested as specified in 4.4.2.

TABLE I. Coated fabric - minimum tensile strengths

Machine direction	9 pounds (4 in. width)
Cross direction	5 pounds (4 in. width)

3.3 Design and construction. The pad shall consist of a single sheet of the coated fabric (3.2.1) 54 ± 2 inches long and 24 +2,-1 inches wide, folded at one end to form a cuff 10 ± 2 inches in length. The cuff shall be formed by heat-sealing the plastic side to the plastic side. The length of the finished pad shall be not less than 43 inches in length. Neither the width nor the length shall vary more than 1/2 inch from the widest to the narrowest point. The pad shall be folded as shown in figure 1.

3.4 Performance.

3.4.1 Sterilization. The pad shall be capable of being sterilized by the ethylene oxide gas method without undergoing any change in material characteristics when tested as specified in 4.4.6.1.


3.4.2 Water permeability. The finished pad shall show no evidence of leakage, when tested as specified in 4.4.3.

3.4.3 Flammability. When tested as specified in 4.4.4, the burning time shall not be less than 3 1/2 seconds.

3.4.4 Surface resistivity or static decay. When tested as specified in 4.4.5, the surface resistivity of the plastic surface shall not exceed 1×10^{11} ohms per square inch or, if the static decay test is employed, the time for the indicated specimen potential to drop to 10% of its maximum value shall not exceed 1/2 second.

3.5 Marking. No marking on the pads is required. Optionally, the words "Prep Pad", the name or registered trademark of the manufacturer, or other descriptive information may be present on the pad, provided it does not occupy a total area greater than 8 square inches and provided the ink used in such marking is indelible in water or in solutions normally used in pre-operating scrubbing.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

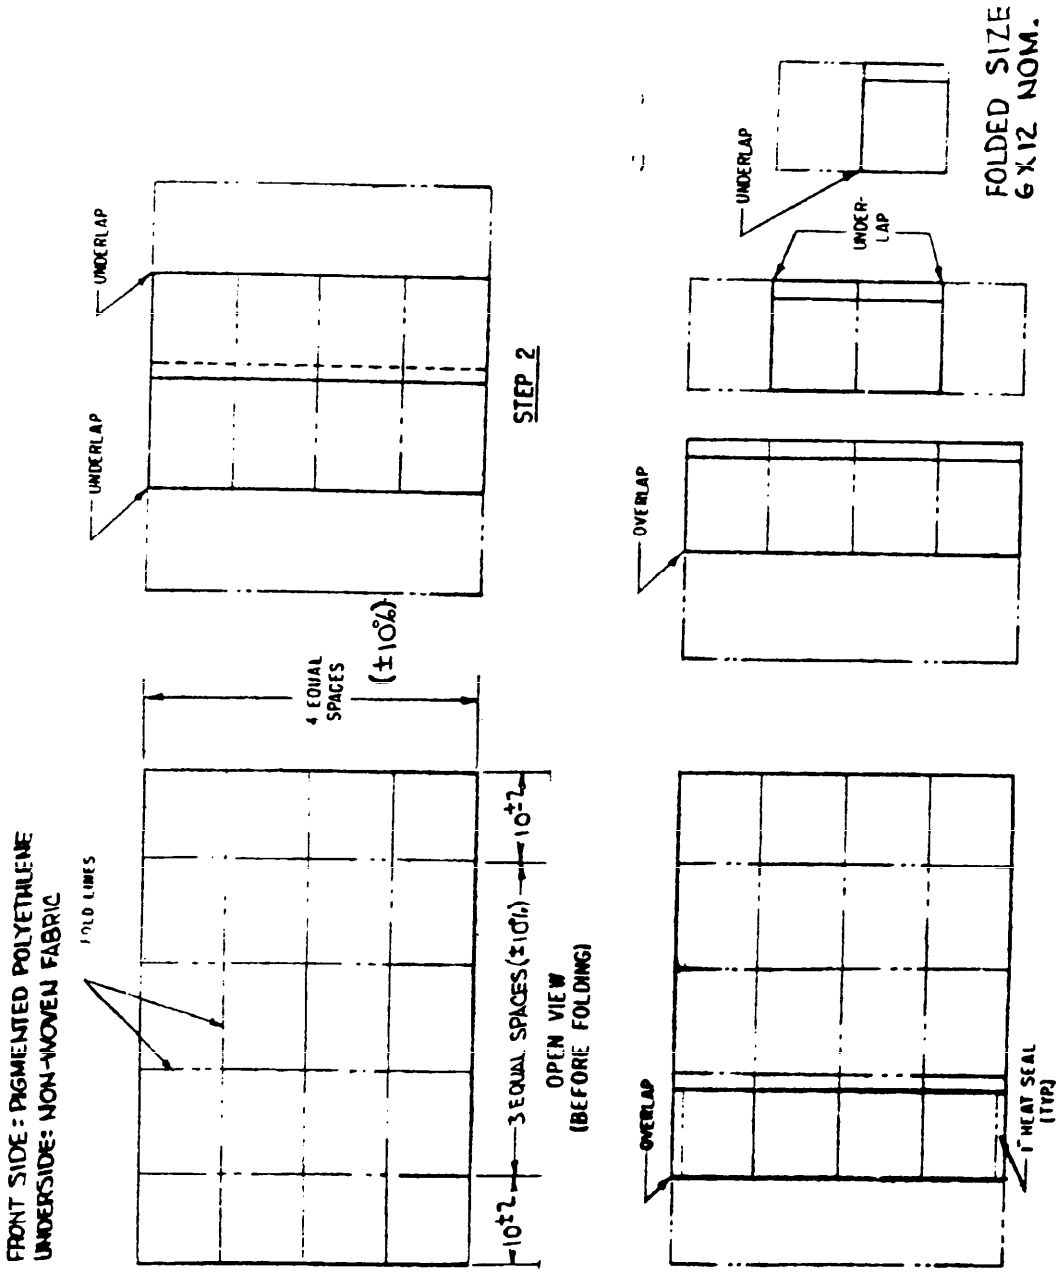

PAD, PRE-OPERATIVE PREPARATION

FIGURE 1

NOTE: ALL DIMENSIONS ARE IN INCHES.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:04Z
Check the source to verify that this is the current version before use.

3.6 Workmanship. Workmanship shall be first class throughout. Pads shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the pad when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and tests of 4.4.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and tests of 4.4 with the exception of 4.4.6.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table II. The unit of product for sampling purposes shall be an individual pad.

TABLE II. Sampling for examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Minor defects	II	4.0
For dimensional examination	S-1	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table III, for an Inspection level of S-1 (except the sterilization test) and AQL of 1.0. The unit of product for sampling purposes shall be one pad, unless otherwise specified in 4.4.

TABLE III. Sampling for tests

Component (Unit of product)	Characteristic	Requirement	Test procedure
Coated fabric or non-woven fabric	Absorbency	3.2.1	4.4.1
Coated fabric	Tensile strength	3.2.1	4.4.2
	Water permeability	3.4.2	4.4.3
	Flammability	3.4.3	4.4.4
	Surface resistivity or static decay	3.4.4	4.4.5
1/Complete pad	Sterilization	3.4.1	4.4.6.1

1/ First article only.

4.3 Examination. The pad shall be examined to determine compliance with all requirements contained in this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table IV. Examination shall not be restricted to the classified possible defects listed below.

TABLE IV. Classification of defects

Categories	Defects
Major	
101	Pad ripped or cut.
102	Cuff not as specified.
103	Plastic backing not continuous.
104	Absorbent layer not continuous.
105	Edges of pad not straight.
Minor	
201	Color of plastic backing not uniform.

4.3.2 Dimensional examination. The pad shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.3.3 Packaging inspection. The inspection of the unit package, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Absorbency. Absorbency shall be determined in accordance with the absorbency time test of ASTM Standard D1117.

4.4.2 Tensile strength. Tests to determine the tensile strength of the coated-fabric in the machine and cross direction shall be conducted in accordance with Test Method 5100 of FED-TEST METHOD STD-191.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

4.4.3 Water permeability. A one foot square section of material shall be selected for test. The material shall be placed, white side down, on top of a beaker or other transparent vessel approximately 6 inches in diameter. The material shall be draped inside of the vessel, a minimum of 2 inches, and the excess secured to the sides of the vessel to hold it in place. Water shall then be poured into the material to a minimum depth of one inch. After 30 minutes the pad shall be examined for evidence of water penetration.

4.4.4 Flammability. Flammability tests shall be conducted in accordance with Test Method 5908 of FED-TEST METHOD STD-191.

4.4.5 Surface resistivity or static decay. Surface resistivity or static decay test shall be conducted in accordance with NFPA 56A.

4.4.6 First article test.

4.4.6.1 Ethylene oxide sterilization. One or more pads shall be sterilized by the ethylene oxide gas method. The sterilized pad(s) shall then undergo the tests of 4.4.1 through 4.4.5. To establish compliance with absorbency requirements, a sufficient sample of non-woven fabric may be sterilized and tested as required in 4.4.1, in lieu of using a complete pad.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One package containing fifty pads as specified, constitutes one unit of issue.

5.1.1.1 Level A.

5.1.1.1.1 Unit packaging. Twenty-five pads shall be packaged in a heavy duty, kraft or plastic bag. Two containers shall be further packaged in a box constructed in accordance with PPP-B-636, type CF, class domestic. Closure of box shall be as specified in the appendix of PPP-B-636.

5.1.1.2 Level C. Units shall be packaged in a manner that will afford adequate protection against deterioration and physical damage during shipment from supply source to the first receiving activity.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A or C as specified (see 6.2).

5.2.1 Level A. Four (4) unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3 style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof as specified in the appendix of PPP-B-636.

5.2.2 Level B. Four (4) unit packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1, or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The packaged units shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking. Each unit package and exterior container shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. The pads are intended for use in military medical facilities.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. When a first article is required (see 3.1, 4.1.2.1 and 6.3).

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of the Armed Services Procurement Regulations. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-457-8193	Pad,Pre-Operative Preparation, 50's

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review Activity:
DOD-MB

Preparing activity:
DLA-DM

Project No. 6530-1415

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS. The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers, vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
MIL-P-37591 PAD, PRE-OPERATIVE PREPARATION, 50's

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:04Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:04Z
Check the source to verify that this is the current version before use.