A-A-51266
9 December 1985

COMMERCIAL ITEM DESCRIPTION

IMPRESSION MATERIAL, DENTAL
(Cartridge Form, Hydrocolloid, Agar Type)

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-I-36878A.

This commercial item description covers a reversible hydrocolloid impression material in cartridges with dispensing needles.

Salient characteristics:

The material shall be a pink or yellow, reversible, hydrocolloid agar in gel form, hermetically sealed in a clear, glass, 1.8 cc cartridge, delivering a minimum of 1.5 cc of material. When prepared in accordance with manufacturer's instructions, shall be suitable for taking accurate dental impressions. The cartridges and needles shall be interchangeable with a standard dental syringe 6515-01-010-8761.

The impression cartridge shall be in accordance with figure 1.

Upon liquefication, the hydrocolloid shall form a smooth consistency and shall be compatible for use with high and low density artificial stones. The temperature at which the liquefied material shall set to a gel shall be not less than 35°C or more than 45°C. The compressive strength shall be not less than 2000 grams per square centimeter (g/cm^2); the strain in compression shall be not less than 4.0% or more than 15.0% between a stress of 100 g/cm^2 and a stress of 1000 g/cm^2. The cartridges shall not rupture or exhibit leakage when boiled for 15 minutes.


In an assembled syringe, depressing plunger shall extrude tempered agar through 19 and 21 gauge needles. The tempered agar shall not have an unpleasant odor or flavor and shall not contain poisonous ingredients in sufficient concentration to be harmful to humana beings when used as directed or in the event of the accidental ingestion of 10 ml.

Each needle shall have a sharpened point at the diaphragm puncturing end and a blunt tip at the dispensing end. Length of both ends of needle shall be 3/8 ± 1/32 inch. The needle cannula shall be made of corrosion-resisting steel of appropriate temper to permit bending and reshaping. Hub shall be threaded to make a suitable fit with syringe. Each needle shall be furnished clean and completely enclosed within a suitable two-piece plastic immediate container designed to facilitate fitting needle to syringe. The plastic containers shall be color coded in contrasting colors to distinguish between 19 and 21-gauge needles.


AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

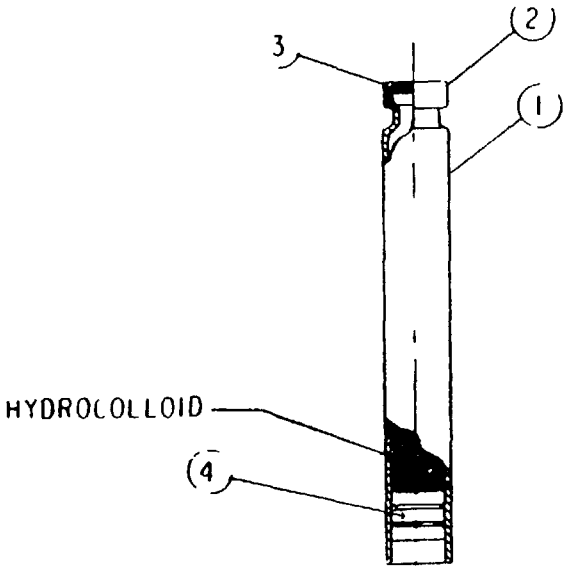

ASSEMBLY

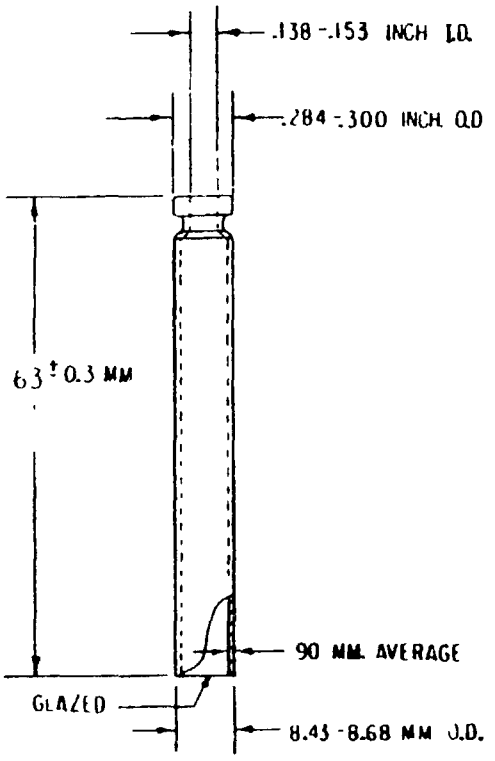

(1) GLASS CARTRIDGE

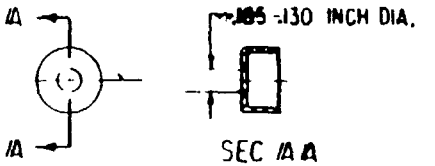

(2) ALUMINUM CAP



(3) RUBBER DIAPHRAGM



(4) RUBBER PLUNGER

IMPRESSION MATERIAL DENTAL CARTRIDGE FORM

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

The package shall consist of forty-eight (48) filled cartridges: twenty-four (24) 19-gauge disposable dispensing needles, twenty-four (24) 21-gauge disposable dispensing needles, and a set of adequate and accurate instructions for use. Specific instructions shall be furnished for enlarging the hole in the nose of the syringe in case the cannula of the 19-gauge needle does not easily pass through the hole.

Workmanship. The impression material shall be clean and free from defects which may affect proper functioning or serviceability.

Unit. Package (PG). One package containing forty-eight cartridges, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one unit package. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted on one unit package from each lot or batch number. Failure of any test shall cause rejection of the lot or batch number.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

Stock Number	Item Identification
6520-00-044-1936	IMPRESSION MATERIAL, Cartridge Form, Hydrocolloid, Agar Type, 48s

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY;

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:
VA-OSS

Project No. 6520-1887

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.