A-A-51279
24 January 1986

COMMERCIAL ITEM DESCRIPTION

CURETTE, SUCTION, UTERINE, Sterile

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers suction curettes designed for vacuum aspiration of uterine contents.

Salient characteristics:

General. Shall be sterile, disposable, semi-rigid curved suction curettes, 8, 10, or 12 mm outer diameter, specifically designed for vacuum aspiration of uterine contents. The curettes shall have thin walls to minimize cervical dilation.

The curettes shall have a proximal end with a male taper which allows secure attachment onto the handle of the disposable tubing collection set. The tubing collection set controls the amount of vacuum delivered to the curettes and will allow the curettes to be rotated.

Material. The curettes shall be made of clear, semi-rigid high quality plastic. The material shall be free from pyrogenicity when tested according to applicable portions of the latest edition of USP. The material shall be non-toxic when tested according to applicable portions of the latest edition of USP for Class IV plastics. The lead content shall not exceed 5 parts per million (ppm).

Characteristics. The curettes shall have an overall length of 7.5 inches and have a rounded tip with a smooth, gentle curve near the middle and an insertion depth marking band at 3.9 to 4.7 inches from the distal end. The curettes shall be in accordance with Figure 1.

Sterility. The curettes shall be sterile when tested in accordance with the applicable portions of the USP. The sterility assurance level shall be 0.0001 as a minimum.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

AMSC N/A
NAVY 3-6-86/1,000

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Workmanship. The curettes shall be processed in such a manner as to be uniform in quality and be free from defects that would affect the life, serviceability, or appearance of the end item.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Material. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Package (PG). One package, containing ten curettes, constitutes one unit. The curettes shall be individually packaged sterile in a peel-open type container capable of maintaining sterility of contents unless the package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 at an Inspection Level of S-2. Dimensional testing shall be a 2.5% AQL. Toxicity, pyrogenicity and lead content testing shall be at a 1.0% AQL. The unit of product for test purposes shall be one package of ten curettes.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

NOTE 1: The following National Stock Numbers are and their respective sizes by outside diameters are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-153-4933	8mm OD
6515-01-185-8836	10mm OD
6515-01-185-8837	12mm OD

NOTE 2: The suction curettes described herein fit the following tubing collection set: 6515-01-156-2452, Collection Tubing Set, Uterine, Plastic, Disposable.

NOTE 3. The suction curettes can be fabricated from cellulose propionate thermoplastic with a Heat Deflection Temperature of 158-165°F at 66 psi in accordance with ASTM D-468.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITY:

VA - OSS

06678

Project No. 6515-3357

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

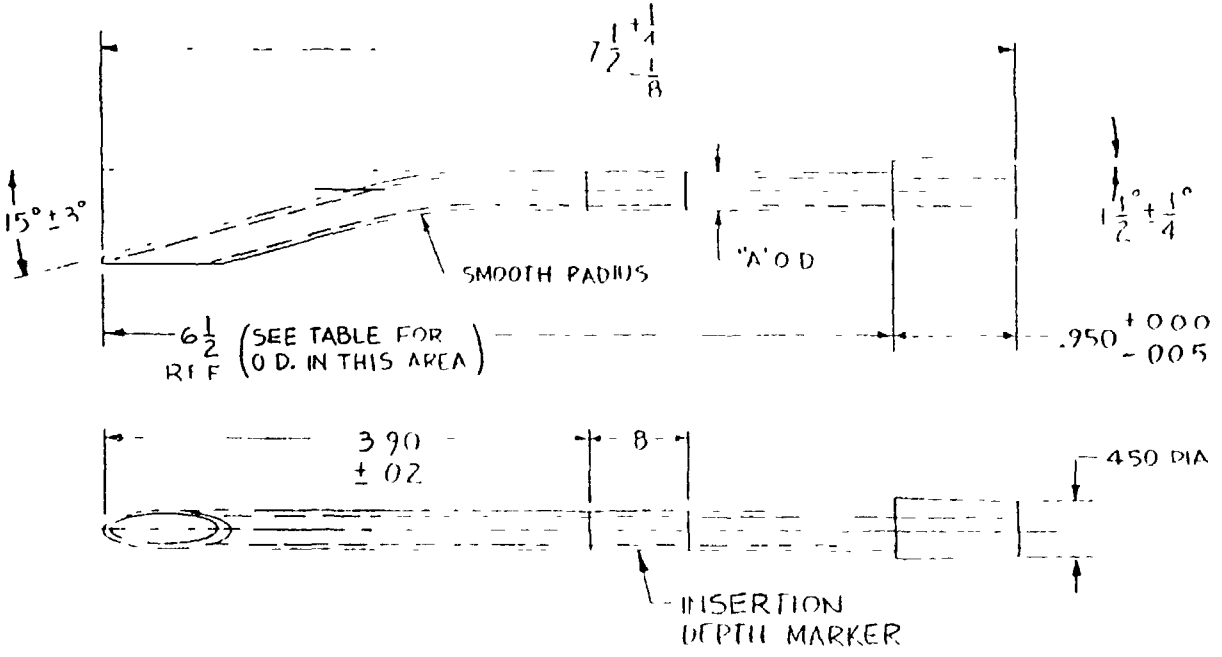

NSN	A (MM) ± .1
6515-01-153-4933	8
6515-01-185-8836	10
6515-01-185-8837	12

NOTE

1. ALL DIMENSIONS IN INCHES UNLESS OTHERWISE SPECIFIED
2. WALL THICKNESS IN 6½" PORTION IS .030" +.010 -.011

FIGURE 1. CURETTE, SUCTION

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.