A-A-51288
18 December 1985

COMMERCIAL ITEM DESCRIPTION

MAGNIFIER, DENTAL OPERATING

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers headband-mounted loupes providing binocular magnification suitable for use in the dental operatory.

Salient characteristics:

The dental operating magnifier shall be headband-mounted loupes providing binocular magnification, so designed as to permit magnification of work leaving both hands free and the wearing of ordinary eyeglasses and bifocals.

The magnifier shall have a headband formed from a curved, flexible, metal strip slotted on one end and having a threaded stud permanently affixed to the opposing end. The ends shall be rounded. The strip, when brought end to end, stud in slot, shall form a lightweight headband shaped to fit, on adjustment, snugly and comfortably around the head. A size adjustment locknut (thumb nut) shall be threaded to fit the stud and shall be positioned on right side of headband. The locknut, with a suitable fiber washer, shall provide for head size adjustments and securing the final adjustment. A removable metal strip, with locating studs permanently affixed at each end, shall be on the inside of brow portion of headband and shall hold replaceable perspiration gauze strips. The gauze shall serve comfort and cleanliness purposes. Four gauze strips shall be furnished with each unit of issue.

A hinge assembly shall be affixed to the front of headband with two suitable flat-headed screws. The assembly shall be angulated downward toward the work area.

A telescoping assembly (inner and outer tube) shall be adjustable for length and locked after adjustment with a suitable locknut. A suitable small wrench shall be furnished with each magnifier for locknut adjustment purposes. The assembly shall have a hinge unit permanently affixed to each end and shall serve as adjustable (up and down) connecting links to the hinge assembly and the lens adjustment hinge of the lens frame. The hinges shall allow raising the magnifying portion above the operator's head when not in use and shall allow the magnifying portion to be folded into the headband area for storage purposes.

Lens frame shall be formed from metal rod and shall be open on both the right and left sides for lens removal and replacement. The lens frame shall be hinged for lens adjustments. The lens frame shall accommodate two 5 diopter crown glass lenses, each with a focal length of approximately 7.8 inches (20 cm), providing a magnification of 2.25X. Suitable grooves shall be ground into two opposite edges of each lens providing secure retention in the frame and easy removal from frame. For design purposes, the magnifier shall be as shown in Figure I.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

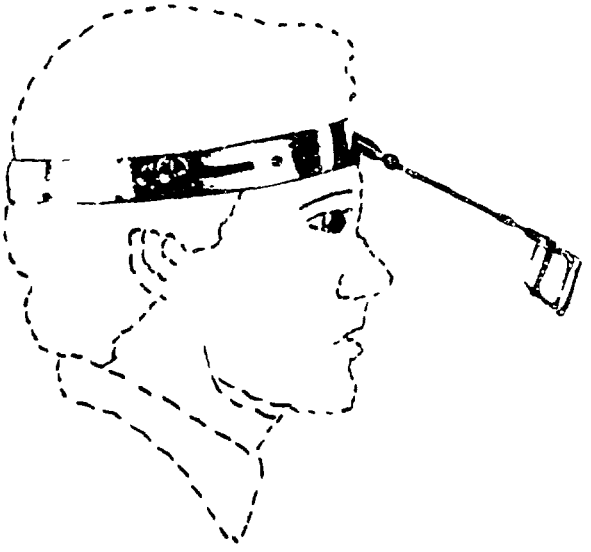


Figure 1. Magnifier, Dental, Operating

The magnifier shown is typical in design and is not intended to restrict or preclude the purchase of magnifiers which are otherwise in accordance with the requirements of this document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Dimensions of the magnifier shall be as follows: Minimum inside circumference of headband shall be 21-1/4 ± 1/4 inches. The total adjustment for size shall be 2-3/4 ± 1/8 inches. The metal strip forming headband shall be 27-3/4 ± 1/4 inches long, 1.0 ± 1/16 inch wide, and 0.024 inch thick. The perspiration band strip shall be 7-7/8 ± 1/8 inches long and shall be of sufficient width and thickness to be suitable for the purpose intended. The lens shall be 32 mm square. The lens thickness shall be 4.2 mm at thin edge and 6.8 mm at mechanical center. The telescoping assembly with hinges shall allow positioning of lens at any angle (up or down) from 4 to 6 inches (10.1 to 15.2 cm) away from eyes.

Material. The headband, hinge assembly, and size adjustment locknut shall be fabricated of aluminum suitable for the purpose intended. The perspiration band, adjustable telescoping assembly, telescoping locknut, lens frame, and lens adjustment hinge shall be fabricated from suitable corrosion-resisting steel. The lenses shall be fabricated of high quality, ophthalmic crown glass and the perspiration band shall be fitted with No. 1 tubular gauze.

Finish. The headband shall have a fine, anodized finish. The hinge assembly and size adjustment locknut shall have a fine, machined finish. The perspiration band shall have a finish suitable for the purpose intended. The remaining corrosion-resisting steel parts shall have a bright finish.

Instructions. Suitable instructions on care and cleaning of the loupes shall be included with each unit of issue.

Workmanship. The magnifier shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One magnifier and four replaceable perspiration gauze strip liners, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for test purposes shall be one magnifier. Unlesss otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5 and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6520-01-082-4898 MAGNIFIER, DENTAL OPERATING, Binocular, Headband-Mounted

Ordering data. Intermediate/exterior package quantities, labeling and marking must be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

CIVIL AGENCY COORDINATING ACTIVITY:
VA-OSS

49053

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

Project No. 6520-1893

Location: S2-12-16

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:53Z
Check the source to verify that this is the current version before use.