A-A-51313
17 March 1986

COMMERCIAL ITEM DESCRIPTION

MASK, ORONASAL

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-A-16040A.

This commercial item description covers four (4) sizes of oronasal masks of two (2) types. These masks are used in conjunction with the standard anesthesia apparatus utilized by the military services.

Salient characteristics:

Masks shall be constructed of molded conductive rubber, and with the exception of the infant size, be reinforced with metallic construction to facilitate reshaping when required. Masks shall be inflatable by means of a valve to control degree of inflation. The exterior surface of the masks shall be coated with conductive synthetic rubber capable of resisting degradation from the effects of ozone and repeated sterilization. All masks shall be equipped with suitable hardware for permitting the use of a headstrap in order to keep the mask firmly on the face of the patient. The overall design and dimensions shall be in accordance with Figure 1 for either Type I or Type II as shown.

All masks shall comply with the National Fire Protection Association (NFPA) Standard 56 A (Standard for the Use of Inhalation Anesthetics) and Underwriters' Laboratories, Inc., (UL) requirements regarding fire and casualty hazards. Evidence that the item meets UL requirements shall be shown by the attachment of a stamp, label, seal or certificate The contracting agency reserves the right to require submission of a laboratory test report used for substantiating conformance.

Masks shall withstand the accelerated aging test described herein without becoming tacky, brittle or decreasing in tensile strength by more than 25 percent.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.
'AMSC N/A'

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

The electrical resistance of the moulded rubber shall not exceed 1 megohm when tested as specified.

Accelerated aging test. Mask shall be subjected to a temperature of 158° ± 2° F. for seven days in an air oven.

Electrical Conductivity test. The resistance between the electrodes shall be measured by any resistance measuring apparatus which has an open circuit, direct voltage of 500 volts.

The four (4) sizes of masks shall be designated as the following:

Sizes	Types
Infant	I & II
Small adult	II
Medium adult	I & II
Large adult	I & II

Workmanship. The cronasal mask shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). Each masks, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one oronasal mask.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers and their respective Item Identifications are covered by this document:

NSN	Item Identification
6515-00-299-8297	MASK, ORONASAL, RESUSCITATOR and ANESTHESIA, LARGE ADULT
6515-00-347-2200	MASK, ORONASAL, RESUSCITATOR and ANESTHESIA, MEDIUM ADULT
6515-00-347-2300	MASK, ORONASAL, RESUSCITATOR, INFANT
6515-00-753-4881	MASK, ORONASAL, RESUSCITATOR, and ANESTHESIA, SMALL ADULT

Custodians:

Army - MD
Navy - MS
Air Force - 03

05245

Preparing Activity:

DoD-MB


Agent:


DLA-DM

Project No. 6515-3388

Location S1-8-22,
NCR(DRUGS)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

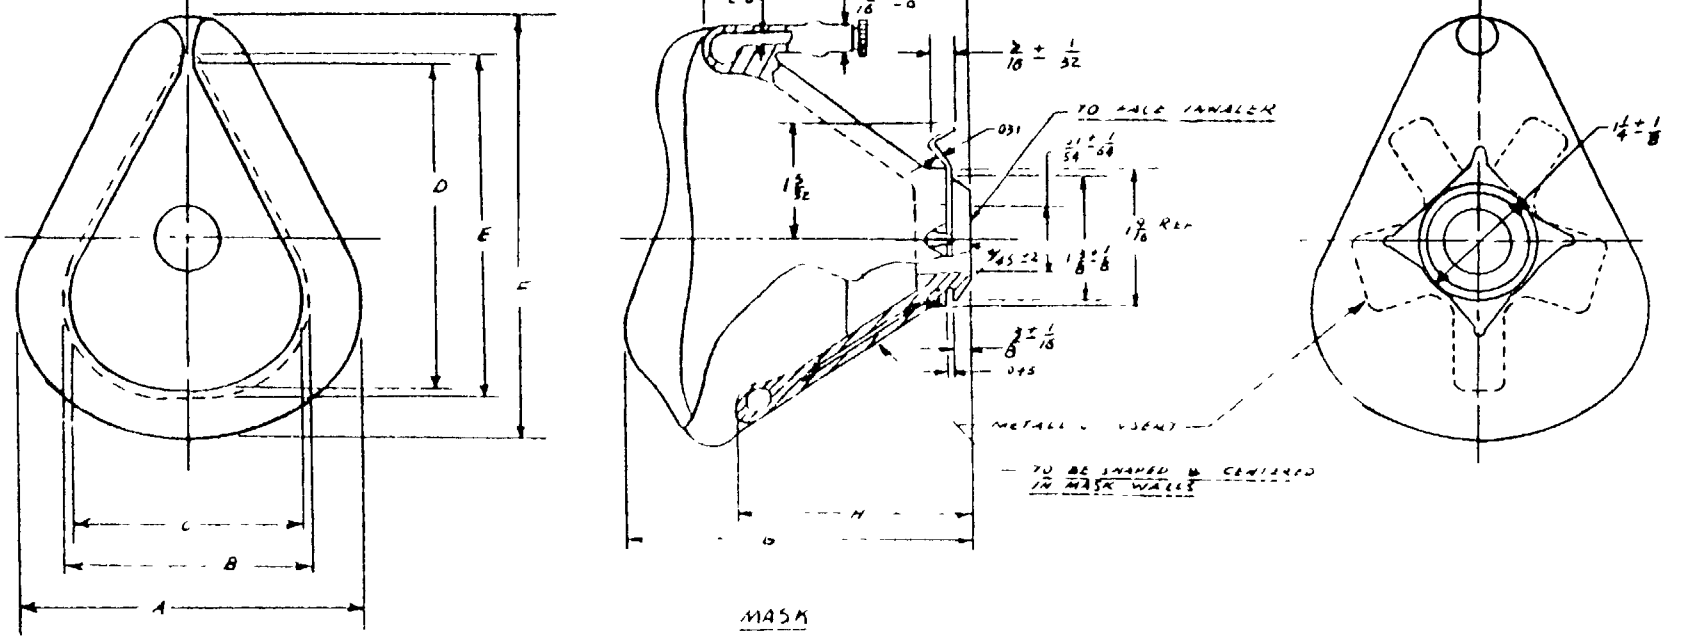

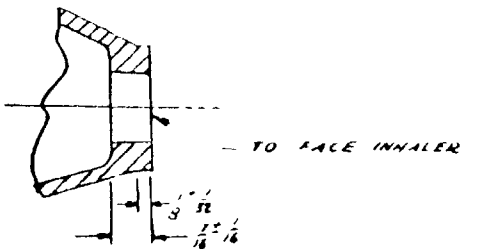

NOTES

1 INFANT MASK SIMILIAR IN DESIGN TO MED & LARGE ADULT MASK EXCEPTING AS SHOWN IE, HOOK RING & METALLIC INSERT NOT REQUIRED

2 SEE TABLE I ON SHEET 3 FOR DIMENSIONS.

TYPE I

FIGURE 1 MASK, ORONASAL (SHEET 1 OF 3)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

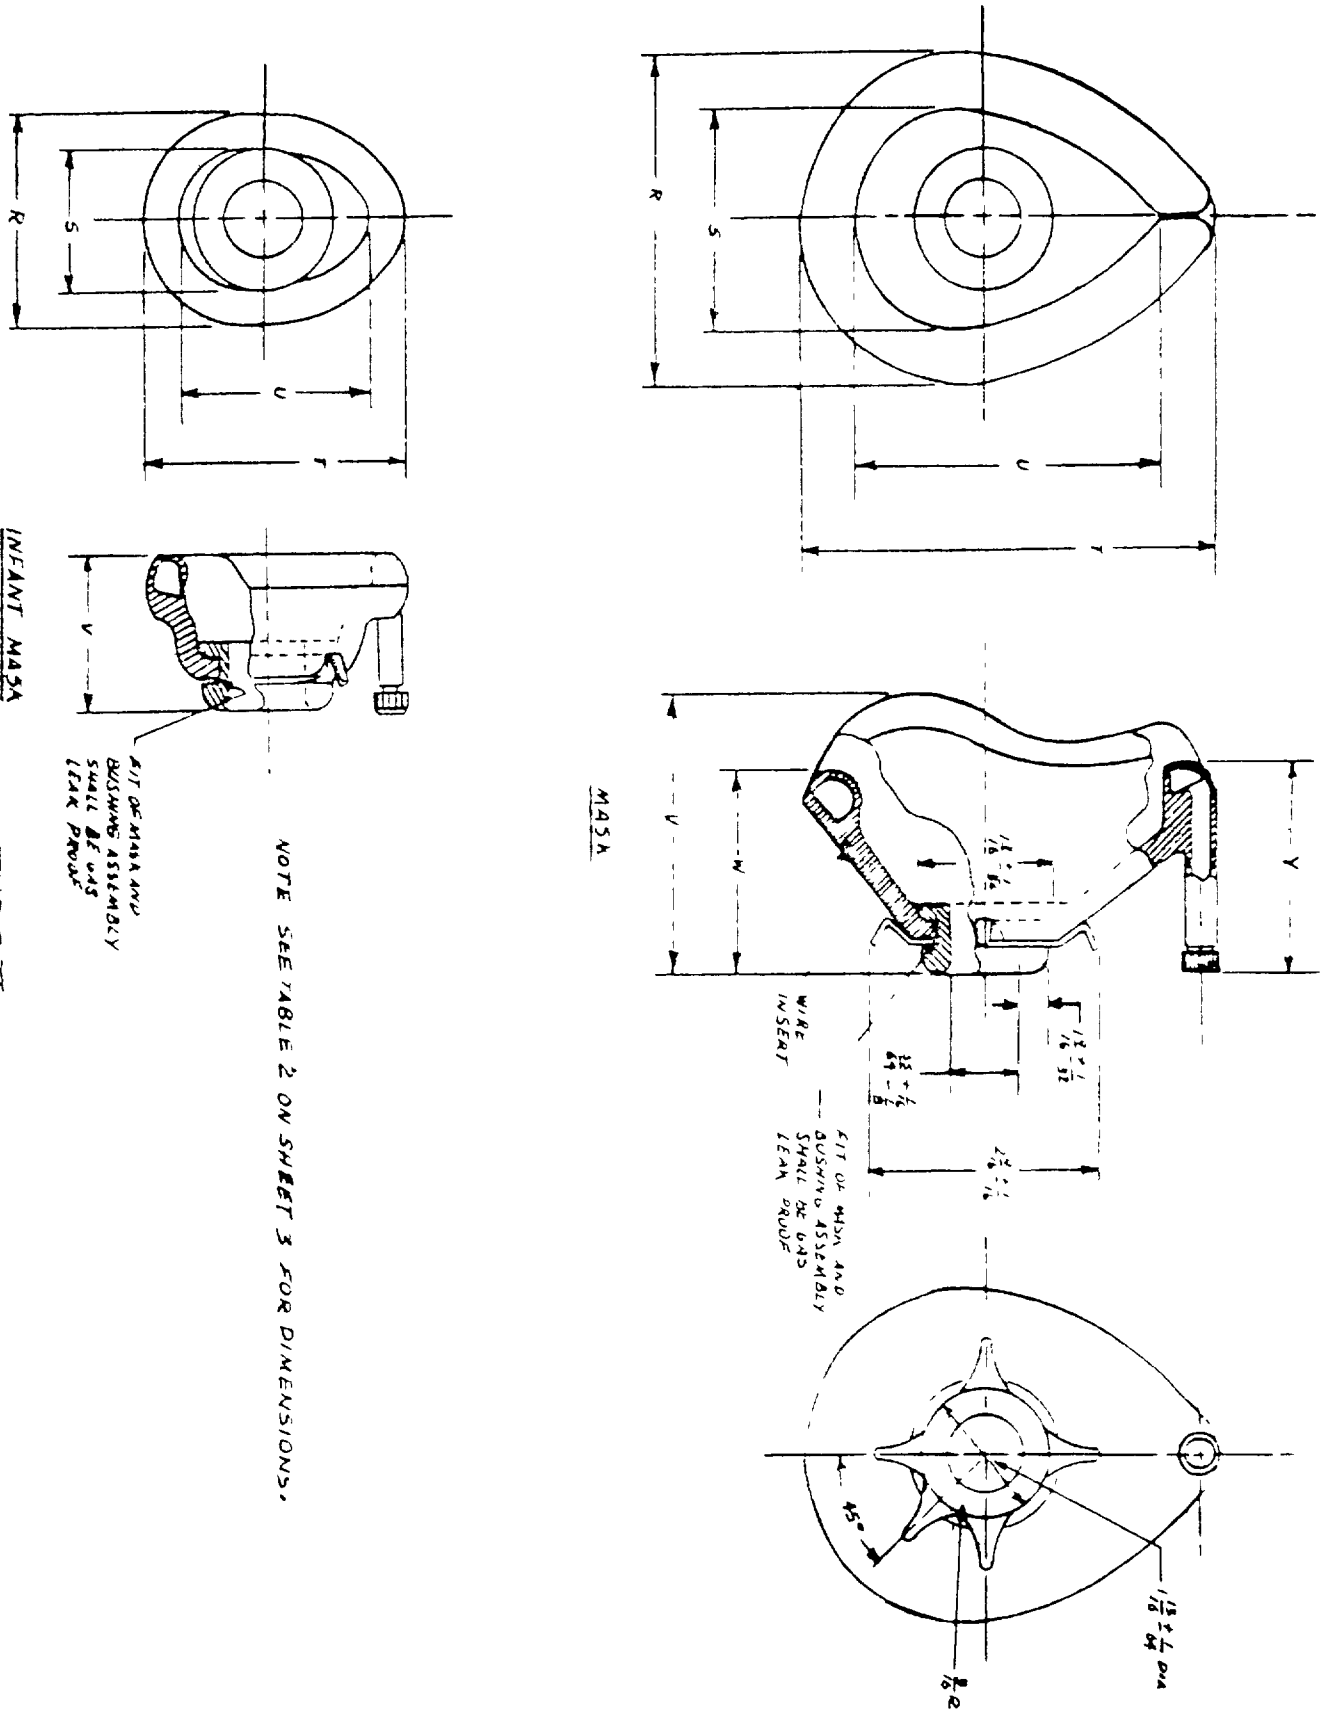


FIGURE 1 MASK, ORONASAL (SHEET 2 of 3)

TYPE II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

											DIMENSIONAL ADJUSTABILITY			
											LENGTH "E"		WIDTH "F"	
STOCK No.	MASK SIZE	A	B	C	D	E	F	G	H	I	MAX	MIN	MAX	MIN
6515-347-2300	2 (MEDIUM ADULT)	3 13/16	2 5/8	2 3/8	3 1/2	3 3/16	4 3/16	5 7/16	2 7/16	2 3/8	4 7/8	4 1/2	4	3 1/2
6515-299-8297	1 (LARGE ADULT)	4 1/4	2 7/8	2 5/8	3 7/16	3 1/4	5	3 3/4	2 3/4	2 7/8	5 1/8	4 3/4	4 1/2	4
6515-347-2340	3 INFANT	2 7/16	1 1/2	1 1/4	1 13/16	2	2 1/8	2 3/16	1 13/16	1 13/16	NON-ADJUSTABLE			
TOLERANCE ON ALL DIMENSIONS - ± 1/4														

TABLE I
TYPE I

									DIMENSIONAL ADJUSTABILITY			
									LENGTH "T"		WIDTH "R"	
FSN	MASK SIZE	R	S	T	U	V	W	Y	MAX	MIN	MAX	MIN
6515-299-8297	LARGE ADULT	4 1/2	2 5/8	4 7/8	3 11/16	3 5/16	2 9/16	2 3/8	5	4 3/4	4 1/2	4
6515-347-2300	MEDIUM ADULT	3 3/4	2 1/2	4 3/8	3 1/2	3 3/16	2 3/8	2 1/4	4 3/4	4 1/2	4	3 1/2
6515-753-9381	SMALL ADULT	3 1/4	2	4 1/8	3 1/4	2 11/16	2 1/16	2	4 3/8	4 1/8	3 1/2	3
TOLERANCE ON ALL DIMENSIONS = ± 1/4												
6515-347-2340	INFANT	2 3/8	1 1/2	2 1/8	2 1/8	1 13/16						
TOLERANCE ON ALL DIMENSIONS - ± 1/4												

TABLE 2
TYPE II

FIGURE 1 (SHEET 3 OF 3)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.