MILITARY SPECIFICATION

LOOP, INOCULATING, LABORATORY, QUANTITATIVE, 0.01 ML

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a breed type, bacteriological inoculating loop, fabricated of rhodium-platinum alloy wire, quantitated to hold 0.01 milliliter (ml.) of liquid inoculum.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids, or request for proposals, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-566 - Boxes, Folding, Paperboard.
PPP-B-636 - Boxes, Shipping, Fiberboard.
PPP-B-676 - Boxes, Setup, Paperboard.

MILITARY

MIL-P-116 - Preservation-packaging, Methods of.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, drawings and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer).

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:13Z
Check the source to verify that this is the currentversion before use.

3. REQUIREMENTS

3.1 Material. The inoculating loop shall be made of rhodium-platinum alloy consisting of 3.5 ± 0.1% rhodium and 96.5 ± 0.1% platinum. Rhodium and platinum content shall be determined as specified in 4.4.1.

3.2 Design and construction. The inoculating loop shall consist of a wire shank with a wire loop at one end. The inoculating loop design is shown on figure 1.

3.3 Weight. The inoculating loop weight shall be not less than 0.90 gms.

3.4 Workmanship. Workmanship shall be first class throughout. The inoculating loop shall be free of defects which detract from its appearance or impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificate of quality. Certificate of quality, supplied by the manufacturer of the platinum-rhodium alloy may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 20261O-21T11:13Z
Check the source to verify that this is the currentversion before use.

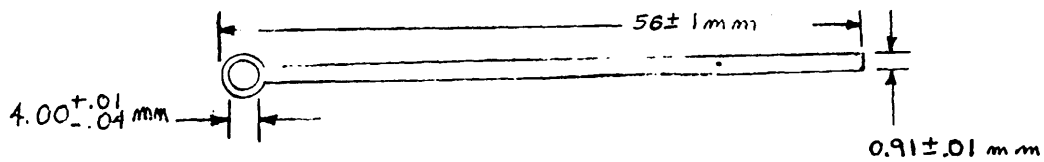


FIGURE 1. Loop, Inoculating, Laboratory, Quantitative 0.01 ML.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:13Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling shall be conducted in accordance with MIL-STD-105 and table I. Unit of product shall be one inoculating loop.

TABLE I. Sampling for examination.

For visual examination	Inspection level	AQL (percent defective)
Major defects	II	1.0
Minor defects	II	2.5
For dimensional examination	S-2	1.0 *

* AQL shall be zero for loop inner diameter dimension.

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table II.

TABLE II. Sampling for tests.

Component (unit of product)	Characteristic	Requirement	Test para.	Inspec. level	AQL
End item	Rhodium content	3.1	4.4.1	S-2	*
End item	Platinum content	3.1	4.4.1	S-2	*

* AQL shall be zero.

4.3 Examination. The inoculating loop shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following table:

TABLE III. Classification of defects.

Categories	Defects *
Major	
101	Loop not free of deformation or scratches.
102	Loop not free of sharp edges or burrs.
103	Loop not free of corrosion or pitting.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:13Z
Check the source to verify that this is the current version before use.

TABLE III. Classification of defects. (cont'd)

Categories	Defects *
Minor	
201	Shank not free of deformation or scratches.
202	Shank not free of sharp edges or burrs.
203	Shank not free of corrosion or pitting.
204	Inoculating loop not free of dirt or foreign material.

* Examination shall not be restricted to the classified possible defects listed.

4.3.2 Dimensional examination. Inoculating loop shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a major defect.

4.3.3 Packaging inspection. The inspection of the preservation-packaging and interior package marking shall be in accordance with the group A and B quality conformance inspection requirements of MIL-P-116. The inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Rhodium and platinum content. Percentage rhodium and platinum content of the inoculating loop shall be determined by chemical analysis or such other methods as may be necessary.

5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning. Loops shall be cleaned in accordance with MIL-P-116, process C-1.

5.1.1.2 Drying. Loops shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative application. Preservatives shall not be used.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:13Z
Check the source to verify that this is the current version before use.

5.1.1.4 Unit packaging. Each loop shall be packed in accordance with MIL-P-116, method III in a sealed kraft or clear polyethylene bag or a suitable size.

5.1.1.5 Intermediate package. Twelve unit packages shall be packaged in a box conforming to PPP-B-566 or PPP-B-676. Closure shall be as specified in the appendix of the applicable box specification.

5.1.2 Level C. Loops shall be clean, dry and individually packaged in a manner that will afford adequate protection against and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Forty-eight (48) intermediate packages (576 units) shall be packed in a shipping container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure, strapping and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Forty-eight (48) intermediate packages (576 units) shall be packed in a shipping container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The packaged loops shall be packed in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier's rules and regulations.

5.3 Marking.

5.3.1 Interior packages. Each unit and intermediate package shall be marked as specified in MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Shipping container. Exterior containers shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. The item covered by this specification is an inoculating loop used to inoculate cultures with .01 ml of inoculating material.

6.2 Ordering data. Procurement document should specify the following:

a. Title, number and date of this specification.
b. National Stock Number (NSN) of item.
c. Selection of applicable levels of packing and packaging.

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:13Z
Check the source to verify that this is the current version before use.

6.2 This specification does not cover all types, classes, grades or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the type normally procured to meet military requirements.

6.3 This specification covers the following item shown in the Federal Supply Catalog:

National Stock No.	Item Identification
6640-01-025-3176	LOOP, INOCULATING, LABORATORY, QUANTITATIVE, 0.01 ml:0.91mm dia. rhodium-platinum alloy wire.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activity:
DoD - MB

Preparing activity:
DLA-DM

Project No. 6640-1011

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:13Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:13Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS: This form is provided to solicit beneficial comments which may improve this document and enhance its use. DoD contractors, government activities, manufacturers, vendors, or other prospective users of the document are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity. A response will be provided to the submitter, when name and address is provided, within 30 days indicating that the 1426 was received and when any appropriate action on it will be completed.

NOTE: This form shall not be used to submit requests for waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

DOCUMENT IDENTIFIER *(Number)* AND TITLE

MIL-L-37661 LOOP, INOCULATING, LABORATORY, QUANTITATIVE, 0.01 ML.

NAME OF ORGANIZATION AND ADDRESS OF SUBMITTER

☐ VENDOR ☐ USER ☐ MANUFACTURER

1. ☐ HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE? ☐ IS ANY PART OF IT TOO RIGID, RESTRICTIVE, LOOSE OR AMBIGUOUS? PLEASE EXPLAIN BELOW.

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDED WORDING CHANGE

C. REASON FOR RECOMMENDED CHANGE(S)

2. REMARKS

SUBMITTED BY *(Printed or typed name and address — Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 OCT 76 1426 EDITION OF 1 JAN 72 WILL BE USED UNTIL EXHAUSTED.

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:13Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

POSTAGE AND FEES PAID

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:13Z
Check the source to verify that this is the current version before use.