MILITARY SPECIFICATION

TABLE, OPERATING, HOSPITAL, PEDESTAL

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a manual major surgical operating table.

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein.

SPECIFICATIONS

FEDERAL

PPP-B-601 - Box, Wood, Cleated-Plywood.
PPP-B-621 - Box, Wood, Nailed and Lock Corner.
PPP-B-636 - Box, Shipping, Fiberboard.
PPP-B-1055 - Barrier Material, Waterproof, Flexible.

MILITARY

MIL-M-7298 - Manual, Technical, Commercial Equipment.
MIL-L-10547 - Liner, Case and Sheet, Overwrap, Water Vaporproof or Waterproof, Flexible.

STANDARDS

FEDERAL

Fed. Test Method Std. No. 151 - Metals; Test Methods.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

(Copies of specifications, standards, drawings, and publications required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN IRON AND STEEL INSTITUTE (AISI)

AISI Steel Products Manual - "Stainless and Heat Resistant Steels".

(Application for copies should be addressed to the American Iron and Steel Institute, 1000 16th Street, N.W., Washington, DC 20036.)

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)

No. 56A Standard for the Use of Inhalation Anesthetics

(Application for copies should be addressed to the National Fire Protection Association, 470 Atlantic Avenue, Boston, MA 02210.)

U. S. DEPARTMENT OF HEALTH, EDUCATION, AND WELFARE,
FOOD AND DRUG ADMINISTRATION (FDA)

Radiation Control for Health and Safety Act and Regulations Promulgated Thereunder.

(Application for copies should be addressed to the Food and Drug Administration, Bureau of Radiological Health, Rockville, MD 20857.)

3. REQUIREMENTS


3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Materials. All materials used in the construction of the operating table shall be suitable in all respects for the purpose intended.

3.2.1 Corrosion-resisting steel. Corrosion-resisting steel shall comply with the AISI 300 series as indicated in the AISI steel products manual when tested as specified in 4.6.1.

3.3 Design and construction. The operating table shall be designed with all parts being closely fitted and shall permit ease of cleaning and shall prevent seepage of oil to the table exterior, and the entrance of liquids, dirt, dust or debris into any of the internal mechanisms. Removable covers, shrouds, and other external appurtenances shall be gasketed or closely fit, and those non-removable, shall be welded and ground smooth to comply with these foregoing conditions. The table shall consist of a mobile base and pedestal (3.3.1), a superstructure (3.3.2) with positioning and control mechanisms for the articulating tabletop, an articulating tabletop (3.3.3) and various required and optional accessories (3.3.4). The operating table shall conform to the illustrations in figure 1.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:19Z
Check the source to verify that this is the currentversion before use.

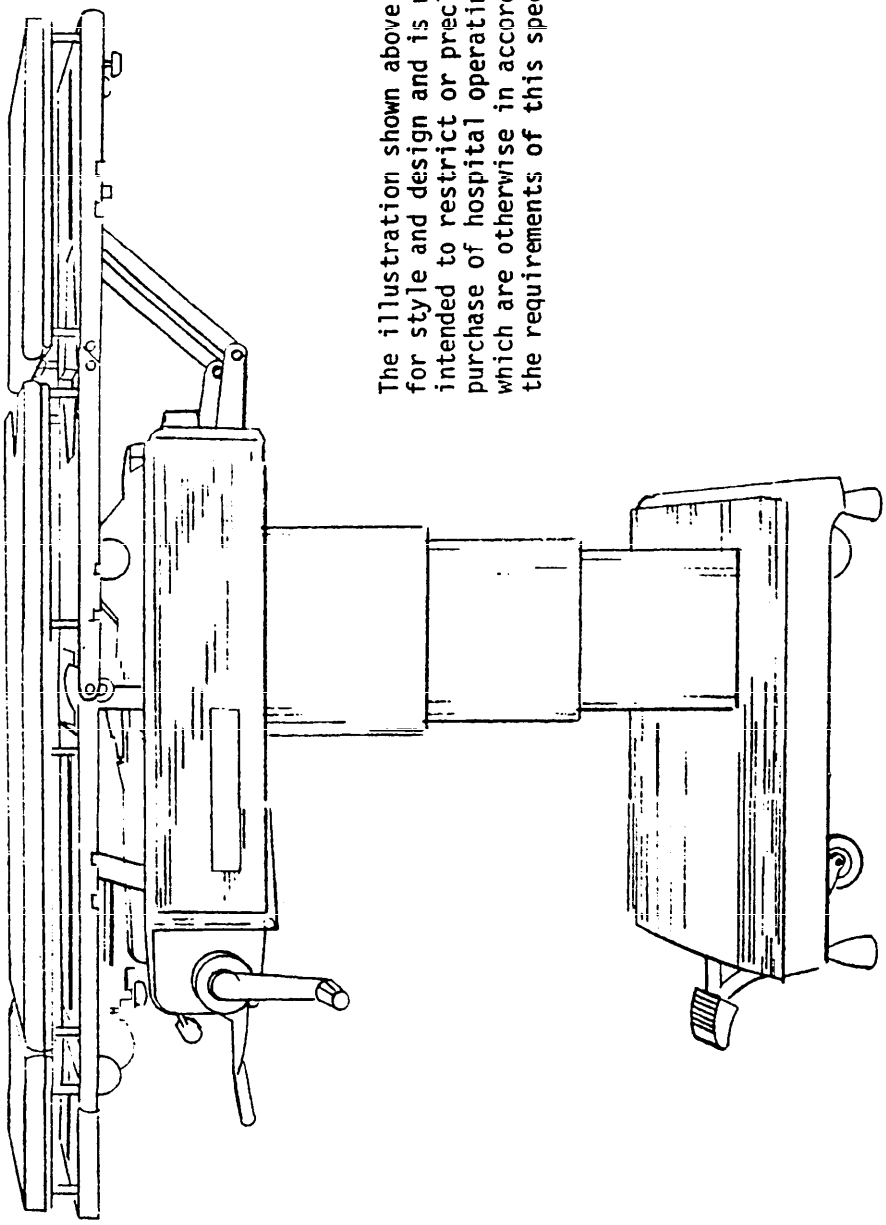

The illustration shown above is typical for style and design and is not intended to restrict or preclude the purchase of hospital operating tables which are otherwise in accordance with the requirements of this specification.

FIGURE 1. Table, operating, hospital, pedestal.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

3.3.1 Mobile base and pedestal. The mobile base shall be of sufficient weight and size to assure that no movement of the table shall occur in any position when supporting a 300 pound patient and shall be covered with corrosion-resisting steel (3.2.1). The equipment base shall be equipped with a patient-grounding receptacle in accordance with NFPA 56A. The base shall be fitted with not less than four electrically-conductive (3.4.5), 3 inch (minimum) diameter, swivel casters and at least four electrically-conductive floor locks which permit compensation for uneven operating room floor surfaces. Casters and floor locks should be inboard of the periphery of the base in order to prohibit interference with personnel movement around the base. A foot pedal, located at the head end of the base, shall control the shift between the caster - supported and floor lock - supported positions. With the floor locks in the down position, there shall be at least a 1/2 inch clearance between the bottom of the base and the floor. The base with the pedestal shall at all times, and in all positions, completely enclose the pedal-actuated hydraulic elevating mechanism. The elevating mechanism shall be enclosed by an inverted telescoping shroud. The bottom section of this shroud shall be fitted, welded to the base cover, and ground smooth, in order to prohibit entrance of liquids. The pump unit shall be a completely sealed system with the oil reservoir pre-filled by the manufacturer. The foot pedal for the elevating mechanism shall be located at the head end of the base for convenient use by the anesthetist. The unit shall be capable of being adjusted to compensate for wear. The foot pedal shall have a 'dead space' between the bottom of the lifting stroke and the start of the lowering position. This makes it necessary to apply additional pressure to the pedal, after a lifting stroke, to move the pedal to the position for lowering the tabletop. The tabletop shall raise and lower smoothly without jarring the patient. The elevating mechanism shall also conform to table I and 3.4.3 for height adjustment of the tabletop and settling requirements, respectively. Also, the pedestal shall prevent rotation of the tabletop with respect to the base. The base shall be so designed that it will allow the blades of a Mayo stand to fit underneath the components of the base, including the hydraulic system at its lowest position.

3.3.2 Superstructure. The superstructure shall be located under, and bearing-mounted to, the seat section of the tabletop. It shall enclose the operating mechanisms for the articulating tabletop sections. Gears and worms shall be machine cut from suitable materials and all load-carrying shafts shall be mounted in antifriction bearings. The superstructure shall carry, at the head end, the hand cranks for controlling the articulating tabletop sections. There shall not be more than three or less than two hand cranks to control the movements of the tabletop. The left-most hand crank, when facing the head end of the superstructure, shall control only the Trendelenburg and reverse Trendelenburg positioning of the tabletop. There shall also be an indicator to show the degree of Trendelenburg, and an indicator showing degrees of lateral tilt. The second crank shall have a function selector associated with it. The function selector shall allow the crank to control the movements of the leg section, the seat section, the back section and flex between the back and seat sections, as desired. The kidney elevator shall be controlled by either the second crank in conjunction with the function selector or by a third crank.

3.3.3 Articulating tabletop. The articulating tabletop shall consist of a leg, seat, and a back section (3.3.3.1), a kidney elevator (3.3.3.2), located between the seat and back sections, and a removable headrest (3.3.3.3). The width of each component of the tabletop, excluding the headrest, shall be at least 20 inches. The length of the tabletop, with the headrest adjusted to a 1 inch clearance space between it and the back section and excluding the footrest, shall be a minimum of 72 inches. Each component of the tabletop shall also conform to the minimum motion requirements of table I.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:19Z
Check the source to verify that this is the current version before use.

3.3.3.1 Leg, seat and back section. The leg, seat, and back section shall consist of a rigid, corrosion-resistant steel framework with a corrosion-resistant steel sheet cover, or cast aluminum, covered with stainless steel sheeting. The seat and back section shall be connected and designed that they will operate together in simultaneous motion to provide flex and reflex. Each section shall have a corrosion-resisting steel siderail running the full length of each side for attaching accessories (3.3.4). The head-end of the leg section and the foot-end of the seat section shall be provided with a perineal cut-out to allow use of a transurethral tray (3.3.4.2.2) without restricting the movement of the leg section of the tabletop. Velcro tape strips shall be applied to the longitudinal centerline of leg, seat, and back sections. The velcro strips shall be located to mate with the tape strips on table top pads and hold them securely without other types of fasteners.

3.3.3.2 Kidney elevator. The kidney elevator shall be constructed of corrosion-resisting steel (3.2.1) and shall adjust to the maximum height specified in table I. When in the lowest position, the top of the kidney elevator shall be either flush with or below the surface of the rest of the tabletop.

3.3.3.3 Headrest. The removable headrest shall be rectangular in shape and shall be constructed of either corrosion-resisting steel (3.2.1) or cast aluminum. The headrest shall be at least 15-3/4 inches wide at the table-end and at least 13-3/4 inches wide at the opposite end. The headrest shall be capable of being adjusted and locked into various angles and shall extend horizontally from the head-end of the back section. The degree of angulation and the range of horizontal extension shall be as specified in table I. The locking mechanism for controlling the angulation of the headrest shall be of the ratchet and locking-bar type. The locking surface of each ratchet tooth shall lie in a radial plane extending through the central axis of the ratchet permitting the free end of the headrest to be raised without actuating the locking-bar but requiring release of the locking-bar before the free end of the headrest can be lowered. The headrest shall also be capable of being attached to the foot-end of, and at a 90° angle to, the leg section to act as a footrest.

3.3.4 Accessories.

3.3.4.1 Required. Each operating table shall be provided with the following removable accessories:

One four-section x-ray-penetrable top (3.3.4.1.1)
Three foam-rubber pads (3.3.4.1.2)
One anesthetist's screen (3.3.4.1.3)
One body restraint strap (3.3.4.1.4)
Two lateral body supports (3.3.4.1.5)
One pair of lithotomy leg holders (3.3.4.1.6)
One pair of padded shoulder supports (3.3.4.1.7)
One pair of wristlets with adjustable holders (3.3.4.1.8)
One intravenous arm board (3.3.4.1.9)
One footrest (3.3.4.1.10)
Support Sockets as required(3.3.4.1.11)

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:19Z
Check the source to verify that this is the current version before use.

3.3.4.1.1 X-ray-penetrable top. The leg, seat, back, and headrest sections of the tabletop (3.3.3) shall each be provided with a removable x-ray-penetrable top which covers the full length and width of the section. Each top shall be capable of being added to, or removed from, the table without the use of tools. Each tabletop section shall be certified and shall be plainly labeled as to being in conformance with the Radiation Control for Health and Safety Act. The space between the x-ray-penetrable top and the tabletop surface shall be sufficient for the insertion, without binding, of a standard 14 by 17 inch cassette. The leg and back sections shall accept the cassette from either side, the head-end or the foot-end. The seat and headrest sections shall accept the cassette from the foot-end and head-end, respectively. A 14 by 17 inch cassette requires a minimum space measuring 18-3/16 inches long, 15-3/16 inches wide and 3/4 inch high. When the width of the headrest is less than that of a 14 by 17 inch cassette (3.3.3.3), the brackets which attach the x-ray-penetrable top to the headrest shall extend outward on the sides in such a manner as to permit the insertion of a 14 by 17 inch cassette from the head-end. The x-ray-penetrable tops, when in place, shall not impede the angulation or adjustment of any section of the tabletop.

3.3.4.1.2 Foam-rubber pads. Three 2-inch thick foam-rubber pads with electrically-conductive rubber covers shall be supplied with each table. One pad shall completely cover the headrest section, one shall completely cover the leg section and the third shall completely cover the back, kidney elevator and seat sections. The pads shall have conductive Velcro tape strips applied to their longitudinal centerlines. These strips shall mate with the strips on the tabletop section and hold the pads securely in place without other fasteners. The electrically-conductive covers for the pads shall conform to the requirements for Reduction in Electrostatic Hazard - Accessories as specified in NFPA 56A.

3.3.4.1.3 Anesthetist's screen. The angulating anesthetist's screen shall be formed from aluminum rod and shall fit into the opening in the angulating section of the dual-function sockets (3.3.4.1.11). The screen shall be capable of use either with or without the x-ray-penetrable top and the foam-rubber pads in place.

3.3.4.1.4 Body-restraint strap. The restraint strap shall be fabricated from a machine-washable, electrically-conductive material which conforms to the requirements for Reduction in Electrostatic Hazard - Accessories as specified in NFPA 56A. The strap shall have two quick-release (aircraft seat-belt type) buckles fabricated of a chrome on nickel-plated metal and shall be suitable for holding a 300 pound patient in place on the operating table throughout the range of table adjustments.

3.3.4.1.5 Lateral body supports. The two lateral body supports shall be formed and contoured to support a patient when the table is in the lateral position. The supports shall slide onto and shall be capable of being secured at any point along the width of the kidney elevator. The supports shall be 3 inches wide with one support being 7 inches long and the other 5 inches long. The ends of the supports shall be rounded. The above dimensions are nominal dimensions.

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:19Z
Check the source to verify that this is the currentversion before use.

3.3.4.1.6 Lithotomy leg holders. Each lithotomy leg holder shall have a strap on one end for supporting the patient's legs and the other end shall fit into a siderail support socket (3.3.4.1.11). The leg holders shall be continuously adjustable about the vertical axis and shall also have a height adjustment. The leg holders shall not interfere with either the X-ray-penetrable top or the foam-rubber pads and shall be supplied in pairs with sockets.

3.3.4.1.7 Shoulder supports. Each shoulder support shall consist of a contoured shoulder rest covered with a removable foam-rubber pad. The shoulder rest shall fit onto, and be capable of being secured at, any point along the length of one leg of an L-shaped bracket. The other leg of the L-shaped bracket shall fit into the non-angulating vertical opening of the dual-function socket (3.3.4.1.11). The bracket shall be long enough so that the shoulder supports will not interfere with use of the X-ray-penetrable top or the foam-rubber pads. Shoulder supports shall be supplied in pairs with dual-function sockets.

3.3.4.1.8 Wristlet with adjustable holder. Each wristlet shall consist of a metal support bracket with a padded wrist restraint strap attached to one end. The other end of the support bracket shall either attach to and slide along the siderail capable of being secured at any point along its length or it shall fit and be secured into a separate siderail support socket (3.3.4.1.11). When a separate socket is needed it shall be supplied with the wristlet. Wristlets shall be supplied in pairs and shall not interfere with either the x-ray-penetrable top or the foam-rubber pads.

3.3.4.1.9 Intravenous arm board. The arm board shall either attach to the siderail or fit into a siderail support socket (3.3.4.1.11). When placed in position, the arm board shall angulate not less than $2\text{-}1/2^{0}$ above the horizontal plane and shall be adjustable, in approximately 10^{0} increments, throughout a range of 180^{0} about the vertical axis. The armboards shall have a removable foam rubber pad with an electrically-conductive rubber cover which conforms to the requirements for Reduction in Electrostatic Hazard - Accessories in accordance with NFPA 56A. The armboard pads shall be held in place by means of conductive Velcro strips to permit easy application and removal for cleaning, and to prevent accidental removal. The arm board shall be capable of being used with the X-ray-penetrable top and the foam-rubber tabletop pads. When a separate siderail support socket is required for the arm board, it shall be supplied.

3.3.4.1.10 Footrest. The removable footrest shall be constructed of corrosion-resisting steel (3.2.1) and shall attach to the foot-end of the leg section of the tabletop in the horizontal position and 90^{0} above the horizontal position. The footrest shall be at least 20 inches wide.

3.3.4.1.11 Support sockets. Each support socket shall be constructed of corrosion-resistant material and shall slide, and be capable of being secured at any point, along the length of the siderail. The sidrails shall be provided with integral, gravity operated locks or equivalent, so that the support sockets will not slide off the ends of the siderail when the table is in steep Trendelenburg or reverse Trendelenburg position. Each dual function socket shall have a locking angulating section with a minimum range of motion of 180^{0} with an opening to accommodate the anesthetist's screen and a non-angulating vertical section with an opening to accommodate a shoulder support. All sockets shall mate freely with their respective accessories.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

3.3.4.2 Optional accessories. Each operating table shall be capable of accommodating the following optional accessories (see 6.2), which must be standard with the manufacturer of the tables.

3.3.4.2.1 Knee-foot rest. The pair of cast aluminum knee-foot rests shall have locking controls to aid in the proper positioning of the patient's legs and shall have straps with buckles with which to hold the patient's legs on the rests.

3.3.4.2.2 Transurethral tray. The transurethral tray shall attach to the table beneath the perineal cutouts on the leg and seat sections (3.3.3.1). The tray shall not interfere with the movement of the leg section. The tray shall contain a tissue-retaining screen and shall have drainage facilities. The tray and the retaining screen shall be formed from corrosion-resisting steel (3.2.1).

3.3.4.2.3 Bierhoff knee crutches. The pair of Bierhoff knee crutches shall have a vertical adjustment and shall have straps to hold the patient's legs in position.

3.3.4.2.4 Headrest.

3.3.4.2.4.1 Neurosurgery-upright position. The neurosurgery-upright position headrest shall be of the padded type. The neurosurgery headrest shall support only the chin and forehead with the patient upright in a modified chair position. The headrest shall be rigid and fully adjustable permitting flexing the head well forward for free unobstructed surgical approach to the occipital region without obstructing oral or nasal administration of anesthetics and without the chin rest contacting the chest, during respiratory movements. The headrest shall permit adjustments for changing the position of the head during surgery to be made beneath drapes away from, and outside of, the sterile field. Frontal support shall consist of removable, adjustable right-hand and left-hand sections.

3.3.4.2.4.2 Neurosurgery-prone position. The neurosurgery-prone position headrest shall be of the padded type. The neurosurgery headrest shall be capable of supporting the patient's head in a prone position, fully adjustable for flexion, extension, and rotation of the cervical spine, with a minimum of 14 inches of horizontal adjustment from the head-end of the back section of the table, with controls placed outside the sterile field and clear of the surgeon's knees.

3.3.4.2.5 Replacement pads. The two occipital and two frontal pads shall have all connecting hardware, be adjustable in every direction, and be suitable for use with the neurosurgery headrests (3.3.4.2.4).

3.3.4.2.6 Arm support. The adjustable arm support shall consist of two hollow aluminum tubes (over which a stockinette can be stretched) connected to a universal ball-joint support which attaches to a siderail support socket (3.3.4.1.11). The universal ball-joint shall allow movement in any plane and shall be capable of being locked into any position.

Source: https://assist.dla.mil -- Downloaded: 20260-21T11:19Z
Check the source to verify that this is the current version before use.

3.4 Performance.

3.4.1 Operation. When the tests specified in 4.3.2 are performed, the operating table shall operate without binding, chatter or slipping. The floor locks, when engaged, shall completely immobilize the table and the foot pedal for the floor locks shall engage positively. The operating table shall conform to the minimum motion requirements as specified in table I when it is immobilized on the floor locks and the tabletop (consisting of headrest, back, seat, kidney elevator and leg sections and excluding the X-ray-penetrable top and foam-rubber pads) is level and 33 inches from the floor. When the table is at a 33-inch elevation and maximum Trendelenburg, the manual controls shall not touch the floor or obstruct the foot pedals.

TABLE I. Minimum motion.

Section	Motion (minimum)	Pedal strokes or hand crank turns required (maximum)
Entire tabletop	Trendelenburg: 20°	15
	Reverse Trendelenburg: 20°	15
	Lateral tilt to right: 10°	
	Lateral tilt to left: 10°	
	Lower to 28 inches above the floor.	
	Raise from 28 inches above the floor to 45 inches above the floor.	58
Headrest	Raise 90° above horizontal.	
	Lower 45° below horizontal.	
	Extend horizontally from back section 1 to 6 inches.	
Kidney elevator	Raise 4-1/2 inches above tabletop.	
	Lower flush with tabletop.	
Back section	Raise head-end 90° above horizontal.	
	Lower head-end 10° below horizontal.	
Seat section	Raise perineal-end 15° above horizontal.	
	Lower perineal-end 20° below horizontal.	
Back and seat sections combined	Flex to form an erect 'V' (at the junction of the two sections) whose included angle is variable from 180° to 140°.	
	Flex to form an inverted 'V' (at the junction of the two sections) whose included angle is variable from 180° to 140°.	
Leg section	Lower 105° below horizontal.	30

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:19Z
Check the source to verify that this is the current version before use.

3.4.2 Headrest rachet and bar strength. The headrest rachet and bar-locking mechanism shall withstand, with no permanent deflection or distortion, a test impact of 400 inch-pounds and 440 inch-pounds performed as specified in 4.6.3.

3.4.3 Settling of elevating mechanism. When tested as specified in 4.6.4 the hydraulic pump unit shall settle no more than 1/16 inch in one hour and 1/8 inch in 24 hours.

3.4.4 Rigidity. With the table at its maximum height, and tested as specified in 4.6.5, there shall be no more than 1/16 inch rotation about the longitudinal axis of the table, 1/8 inch rotation about the vertical axis and 1 inch rotation about the transverse axis.

3.4.5 Electrical conductivity. The completely assembled operating table shall meet the conductivity requirements of NFPA 56A.

3.5 Finish. All exposed corrosion-resisting steel parts shall be given a No. 4 commercial finish. All other steel parts shall either have a chrome on nickel-plated finish or a baked enamel finish. All other metal parts shall have a baked enamel finish. The enamel shall be applied in two coats. Each coat shall be baked on in accordance with the paint manufacturer's instructions. The color of the enamel shall be silver lustre or dark gray. All finishes shall be clean, smooth and uniform and free from blistered, peeled, scratched and uncoated areas.

3.6 Identification marking. Each operating table shall be marked permanently and legibly with the following:

Contract or purchase order number.
Name or registered trademark of the manufacturer.
Manufacturer's model number.
National Stock Number.
Manufacturer's serial number.

3.7 Service data. The contractor shall furnish, with each table, two copies each of a technical manual which contains completely instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request to the Contracting Officer. Waiver of submission of drafts and submission of 15 additional copies shall be at the option of the Government.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

3.8 Workmanship. Workmanship shall be first class throughout. Tables shall be free from defects which detract from their appearance or may impair their serviceability. All burrs and sharp edges shall be removed.

3.8.1 Welding. Welding shall be durable, sound in every detail and in accordance with the latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive splatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

4.1.2.1.1 First article inspection. First article inspection shall be performed on operating tables when a first article sample is required (see 3.1). This inspection shall include examination of 4.4 and tests of 4.6.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.4 and tests of 4.6.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/ material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Inspection lot.

4.2.1 Raw materials. An inspection lot for raw material inspection shall be all material produced under the same conditions and controlled to the degree that uniformity of product within the designated lot can be assured. Lot identification of the raw material by the manufacturer is one method of control, as cited above, which is considered acceptable.

4.2.2 End product. An inspection lot for inspection of end product shall consist of all operating tables of the same type produced under essentially the same conditions and offered for inspection at one time.

4.3 Sampling.

4.3.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table II. The unit of product for sampling purposes shall be one table.

TABLE II. Sampling for examination.

	Inspection level	AQL (defects per hundred units)
For viaual examination		
Major defects	II	1.0
Total defects (Major and Minor combined)	II	4.0
For dimensional examination	S-1	2.5

Source: https://assist.dla.mil -- Downloaded: 2026l0-21T11:19Z
Check the source to verify that this is the currentversion before use.

4.3.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table III, for an Inspection level of 100% and an acceptance number of zero. The unit of product for sampling purposes shall be one table. The 24 hour settling test of the elevating mechanism shall be performed on only one unit per lot (4.2.2).

TABLE III. Sampling for tests.

Characteristic	Requirement	Test procedure
Operation	3.4.1	4.6.2
Headrest rachet and bar strength	3.4.2	4.6.3
Settling of elevating mechanism	3.4.3	4.6.4
Rigidity	3.4.4	4.6.5
Electrical conductivity	3.4.5	4.6.6

4.3.3 Raw materials. Each lot of each metal used in the manufacture of the operating tables shall be selected for chemical analysis as specified in 4.6.1.

4.4 Examination. The operating tables shall be examined to determine compliance with all requirements contained in this specification.

4.4.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table IV. Examination shall not be restricted to the classified possible defects listed below.

TABLE IV. Classification of defects.

Categories	Defects
Major	
101	Table not complete with all required component parts and accessories.
102	Casters not as specified.
103	Metal and cast parts not free of cracks, ruptures, and deformed sections.
104	Exposed and accessible edges and corners not free of burrs and sharpness.
105	Welds not sound, smoothly blended, and free of flux, discoloration, and spatter.
106	Mating parts not properly fitted, assembled, and secured.
107	Packaged parts and subassemblies not clearly identified as to contents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

TABLE IV. Classification of defects. (continued)

Categories	Defects
Minor	
201	Painted and plated surfaces not free of blisters, and peeled, scratched, or uncoated areas.
202	Corrosion-resisting steel surfaces not smooth and of uniform finish.
203	Color of enamel finish not as specified.
204	Identification marking (nameplate) not present or complete with specified information.
205	Surface of tabletop and exterior surfaces of unit not clean and free of dirt, oil, grease, chips, and foreign matter.
206	Service data in duplicate not included.
207	Headrest, when in down position, interferes with the operation of the back section.
208	Any enameled surface scratched as a result of contact with another surface of the table during any of the articulations.

4.4.2 Dimensional examination. The operating tables shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.5 Packaging inspection. The inspection of the unit packaging, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.6 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.6.1 Chemical composition. Four ounces from each lot of material shall be tested in accordance with Fed. Test Method Std. 151.

4.6.2 Operation.

4.6.2.1 Unloaded.

4.6.2.1.1 Floor locks and swivel casters. Depress the foot-pedal to place the table in the floor lock-supported position. Depress the pedal once again to place the table in the caster-supported position. Repeat a total of five times.

4.6.2.1.2 Minimum motion. Manipulate the tabletop through all of its articulations: raise entire tabletop; lower entire tabletop; Trendelenburg, reverse Trendelenburg; lateral tilt left, lateral tilt right; headrest, back section, seat section and leg section motions; and combination back and seat section motions. Repeat a total of five times.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:19Z
Check the source to verify that this is the currentversion before use.

4.6.2.2 Loaded. Place a 300 pound (136kg) dummy patient on the table and repeat the tests specified in 4.6.2.1.1 and 4.6.2.1.2. The dummy shall consist of a four-section bag with the following weight distribution: 25 pounds (11.4kg) on the head section; 100 pounds (45.4kg) on the back section; 140 pounds (63.6kg) on the seat section; and 35 pounds (15.9kg) on the foot section. The table shall meet the requirements of 3.4.1.

4.6.3 Headrest rachet and bar strength. The headrest rachet and bar-locking mechanism shall be tested in accordance with step numbers one to five for a 400 inch-pound test impact and step number six for a 440 inch-pound test impact.

1. Attach the headrest to the head-end of the back section and lock it into the horizontal position.
2. Suspend a 20 lb. weight from the headrest, by means of a C-clamp and a length of chain, in line with the extreme edge of the headrest at a 9-3/4 inch distance from the headrest pivot shaft centerline.
3. While the weight is hanging freely from the headrest, measure height of weight above floor.
4. Raise the weight the required drop distance of 20 inches and loop suspend the chain. The two ends of the chain loop shall be tied together with cord.
5. Release the weight by burning through the holding cord.
6. Repeat the complete test procedure using a 22 inch drop distance.

4.6.4 Settling of elevating mechanism. Place the three hundred pound dummy patient (4.6.2.2) on the operating table and then set the table at its maximum height. Measure the initial height of the tabletop, the height after one hour and the height after twenty-four hours (4.3.2).

4.6.5 Rigidity. With the table adjusted to its maximum height, the following three tests shall be performed.

4.6.5.1 Rotation about the longitudinal axis. Hang fifty pounds from one seat section siderail approximately half way along the length of the seat section. Measure the height from the floor of the edge of the seat section of the tabletop most near to where the weight is suspended. Shift the weight to approximately the same position at the other side of the table. Measure the height of the edge of the seat section from the floor at the same place where the first measurement was taken. Take the difference between the two measurements.

4.6.5.2 Rotation about the vertical axis. Measure the horizontal movement of the end of the siderail most near to the foot-end of the table when a fifty pound horizontal pull is exerted at a 90^{0} angle to the end of the siderail most near the head-end of the table.

4.6.5.3 Rotation about the transverse axis. Hang fifty pounds from the center edge of the free-end of the headrest. Measure the height of this point of attachment of the weight above the floor. Shift the weight to the center edge of the foot-end of the leg section. Again measure the height of the center edge of the free-end of the headrest from the floor. Take the difference between the two measurements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

4.6.6 Electrical conductivity. The completely assembled operating table shall be tested using the equipment and procedure described in Reduction in Electrostatic Hazard of NFPA 56A.

5. PACKAGING

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A. Each unit shall be disassembled as far as is practicable. All exterior finished surfaces of the table shall be protected by wrapping with kraft paper or other suitable material and cushioned with corrugated fiberboard, polyurethane or other suitable cushioning material. The unit shall be protected in such a manner to insure against marring, scratching or damage to the unit. Disassembled parts and accessories shall be packaged in one or more fiberboard or wood boxes conforming to PPP-B-601, PPP-B-621 or PPP-B-636 class weather-resistant. Components shall be wrapped in kraft paper or other suitable noncorrosive material and cushioned within the containers in such a manner to prevent damage during shipping and handling. Closure shall be as specified in the appendix of the applicable box specification. Wood boxes shall be lined with a waterproof case liner conforming to MIL-L-10547. Fiberboard boxes shall be waterproofed as specified in PPP-B-636.

5.1.2 Level C. Each table along with component parts shall be packaged in accordance with the contractor's commercial practice.

5.2 Packing. Packing shall be level A or C as specified (see 6.2).

5.2.1 Level A. Each unit packaged as specified in 5.1.1 shall be packed in a shipping container conforming to PPP-B-601, overseas type or PPP-B-621, class 2. The table shall be adequately secured within the container by use of blocking and bracing or by other suitable means to prevent shifting, damage or marring of surfaces. Boxes containing disassembled components and accessories shall be secured to the base of the shipping container. All panels of the shipping container except the base shall be lined with barrier material conforming to PPP-B-1055, class E2. Ths shipping container shall be provided with skids of not less than 1-1/2 inches in thickness applied crosswise of the base so positioned as to facilitate handling with a forklift and to maintain the unit in an upright position. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level C. Each packaged table shall be packed in a shipping container that will afford adequate protection against corrosion, deterioration and damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the carriers rules and regulations.

5.3 Marking. Interior packages shall be marked to identify contents and the shipping container shall be marked as specified in MIL-STD-129.

6. NOTES

6.1 Intended use. The operating table covered by this specification is intended for use in the military surgical service.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. Optional accessories required (see 3.3.4.2).
d. When a first article is required (see 3.1, 4.1.2.1 and 6.3).

6.3 First article. When a first article is required, it shall be tested under the appropriate provisions of the Defense Acquisition Regulations (ASPR). The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-142-8795	TABLE, OPERATING, HOSPITAL, PEDESTAL

6.5 Replacement electrically-conductive foam-rubber pads (see 3.3.4.1.2) appear in the Federal Supply Catalog as follows:

National Stock Number	Item Identification
6530-00-709-9250	PAD, OPERATING TABLE, FOAM-RUBBER

Military custodians:
Army - MD
Navy - MS
Air Force - 03

Review activity:
DoD - MB

Preparing activity:
DLA-DM

Project No. 6530-1425

Source: https://assist.dla.mil -- Downloaded: 202640-21T11:19Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS: This form is provided to solicit beneficial comments which may improve this document and enhance its use. DoD contractors, government activities, manufacturers, vendors, or other prospective users of the document are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity. A response will be provided to the submitter, when name and address is provided, within 30 days indicating that the 1426 was received and when any appropriate action on it will be completed.

NOTE: This form shall not be used to submit requests for waivers, deviations or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

DOCUMENT IDENTIFIER *(Number)* AND TITLE

MIL-T-37702 TABLE, OPERATING, HOSPITAL, PEDESTAL

NAME OF ORGANIZATION AND ADDRESS OF SUBMITTER

☐ VENDOR ☐ USER ☐ MANUFACTURER

1. ☐ HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE? ☐ IS ANY PART OF IT TOO RIGID, RESTRICTIVE, LOOSE OR AMBIGUOUS? PLEASE EXPLAIN BELOW.

A. GIVE PARAGRAPH NUMBER AND WORDING

B. RECOMMENDED WORDING CHANGE

C. REASON FOR RECOMMENDED CHANGE(S)

2. REMARKS

SUBMITTED BY *(Printed or typed name and address — Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 OCT 76 1426 EDITION OF 1 JAN 72 WILL BE USED UNTIL EXHAUSTED.

Source: https://assist.dla.mil -- Downloaded: 202610-21T11:19Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

POSTAGE AND FEES PAID

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

DEFENSE PERSONNEL SUPPORT CENTER
DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T11:19Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL