INCH-POUND

MIL-D-26392C (USAF)
28 October 1994
SUPERSEDING
MIL-D-26392B (USAF)
30 SEPTEMBER 1980

MILITARY SPECIFICATION

DUMMY CONVERTERS, LIQUID OXYGEN INDICATOR SYSTEM

10 LITER CRU-23/A AND 25 LITER CRU-24/A

This specification is approved for use by the Department of the Air Force and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers two types of dummy converters (electrical capacitor) having a capacitance equivalent to an empty, 10-liter and 25-liter liquid oxygen converter, with respect to a capacitance type quantity gauging system.

1.2 Classification. The converters shall be classified as follows (see 6.6):

Type	Designation	Liters
1	CRU-23/A	10
2	CRU-24/A	25

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1. Specifications, standards, and handbooks. The following specifications, standards, and handbooks form a part of this document to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation (see 6.2).

SPECIFICATION

FEDERAL

PPP-B-601	Boxes, Wood, Cleated-Plywood
PPP-C-1797	Cushioning Material, Resilient, Low Density, Unicellular, Polypropylene Foam

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Oklahoma City Air Logistics Center/TICLA, Tinker AFB OK 73145-5990 by using the Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC N/A FSC 1660

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

MILITARY

MIL-P-116	Preservation Method Of
MIL-B-121	Barrier Material, Greaseproofed, Waterproofed, Flexible
MIL-B-131	Barrier Material, Watervaporproof, Flexible, Heat-Sealable
MIL-C-25516	Connectors, Electrical, Miniature, Coaxial, Environment Resistant Type, General Specification For

STANDARDS

MILITARY

MIL-STD-100	Engineering Drawing Practices
MIL-STD-129	Marking For Shipment And Storage
MIL-STD-130	Identification Marking Of US Military Property
MIL-STD-721	Definitions Of Terms For Reliability, Maintainability
MIL-STD-781	Reliability Testing For Engineering Development, Qualification, & Production
MIL-STD-810	Environmental Test Methods & Engineering Guidelines
MIL-STD-831	Test Reports, Preparation Of
MIL-STD-889	Dissimilar Metals
MIL-STD-970	Standards & Specifications Order Of Preference For The Selection Of

(Unless otherwise indicated, copies of federal and military specifications, standards, and handbooks are available from the Standardization Document Order Desk, 700 Robbins Ave, Building #4, Section D, Philadelphia, PA 19111-5094.)

2.1.2 Other Government documents, drawings, and publications. The following other Government documents, drawings, and publications form a part of this document to the extent specified herein. Unless otherwise specified, the issues are those cited in the solicitation.

DRAWING

AIR FORCE

8148650	Document - Cleaning, Inspection and Packaging of Breathing Oxygen Equipment

(Applications for copies should be addressed to OC-ALC/TICLA, 3001 Staff Drive, Tinker AFB, OK 73145-5990)

2.2 Non-Government publications. The following document(s) form a part of this document to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DODISS cited in the solicitation. Unless otherwise specified, the issues of documents not listed in the DODISS are the issues of the documents cited in the solicitation (see 6.2).

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM D5118/D5118M	Standard Practice For Fabrication Of Fiberboard Shipping Box
ASTM D1974	Standard Practice For Methods Of Closing, Sealing, And Reinforcing Fiberboard Shipping Containers

(Applications for copies should be addressed to: ASTM, 1916 Race St, Philadelphia, PA 19103.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

(Non-Government standards and other publications are normally available from the organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this document and the references cited herein (except for related associated detail specifications, specification sheets, or MS standards), the text of this document takes precedence. Nothing in this document, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 First article. When specified (see 6.2), a sample shall be subjected to first article inspection (see 6.4) in accordance with 4.4.

3.2 Selection of specifications and standards. Specifications and standards for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-970.

3.3 Dissimilar metals. Unless suitably protected against electrolytic corrosion, dissimilar metals shall not be used in intimate contact with each other. Dissimilar metals are defined in MIL-STD-889.

3.3.1 Reclaimed materials. The use of reclaimed materials shall be encouraged to the maximum extent possible without jeopardizing the end use of the item.

3.4 Design and construction. The design and construction of the dummy converter shall be in accordance with figure 1 or figure 2 as specified. The complete dummy converter shall consist of the following components:

Capacitor
Case
Electrical connectors
Mounting plate
Protective covers

3.4.1 Capacitor. The capacitor for the type 1 shall have an electrical capacitance of 123.5 $\pm$ 1.0 Picofarads (PF), and the type 2 shall have an electrical capacitance of 303.5 $\pm$2.5PF. The rated voltage of the capacitors shall be 110 volts.

3.4.2 Case. The case shall conform to the configuration and dimensions of figure 1 or figure 2 as specified. The case shall provide a moisture tight seal for the capacitor. The case shall be made of corrosion-resistant material or from material that has been suitably protected against corrosion. The use of any protective coating that will crack, chip, or scale with age or extremes of atmospheric conditions shall be avoided. The case may be round or square and shall be centered on the mounting plate.

3.4.3 Electrical connectors. The electrical connectors shall be as shown on figure 1 and figure 2, and they shall be of the Jack Body Type. Receptacle ends shall be equivalent to MIL-C-25516 connectors.

3.4.4 Mounting plate. The mounting plate shall conform to the configuration and dimensions of figure 1 or figure 2 as specified. The mounting plate shall be made of corrosion-resistant material or from material that has been suitably protected against corrosion. The use of any protective coating that will crack, chip, or scale with age or extremes of atmospheric conditions shall be avoided.

3.4.5 Protective covers. The protective covers shall be constructed similar to the couplings of MIL-C-25516 and shall connect and disconnect in a similar manner. They shall electrically and mechanically protect the electrical connectors. They shall be secured to the mounting plate with a metal beaded chain or similar devise capable of withstanding a pull of 40 pounds force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

3.5 PERFORMANCE

3.5.1 Capacitance at room temperature. The capacitance at room temperature for the type 1 shall be 123.5 ±1.0 PF and the type 2 shall be 303.5 ±2.5PF (see 4.6.2).

3.5.2 Capacitance at low temperature. The capacitance at -65°F shall remain within the tolerance specified for room temperature (see 4.6.3).

3.5.3 Capacitance at high temperature. The capacitance at 260°F shall remain within the tolerance specified for room temperature (see 4.6.4).

3.5.4 Immersion (leakage). The case shall not leak when the dummy converter is subjected to the immersion (leakage) test (see 4.6.5).

3.5.5 Reliability. The dummy converter shall have a specified mean-time-between-failures (MTBF) of not less than 300 hours at the 90 per cent lower confidence limit. (This is equivalent to minimum acceptable MTBF of 200 hours, and to a reliability of .9933 for 2-hour mission) (see 4.6.6)

3.5.5.1 Service life. The service life of the dummy converter shall be not less than 1,000 hours before wear out failures occur or the dummy converter fails to meet the specified MTBF.

3.5.6 Maintainability. Mean corrective maintenance task time as defined in MIL-STD-721, shall not exceed one hour (see 4.6.7).

3.6 Weight. The complete dummy converter shall not weigh more than 0.25 pound.

3.7 Identification of product. The dummy converters shall be marked for identification in accordance with MIL-STD-130 and shall include the following information as applicable:

Dummy Converter	Dummy Converter
10 Liter	25 Liter
M26392-1	M26392-2
Type CRU-23/A	Type CRU-24/A
Manufacturer's Part Number*	Manufacturer's Part Number*
Contract Number*	Contract Number*
Manufacturer's Name or Trademark*	Manufacturer's Name or Trademark*

*The manufacturer shall include applicable information.

3.8 Interchangeability. All parts having the same manufacturer's part number shall be directly and completely interchangeable with each other with respect to installation and performance. Changes in manufacturer's part numbers shall be governed by the drawing number requirements of MIL-STD-100.

3.9 Workmanship. The dummy converters shall be uniform in quality and shall be free from irregularities or defects which could adversely affect safety, performance, reliability, or durability. The converters shall be free of oil, grease, fuel, water, dust, dirt, or any other foreign matter.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements (examinations and tests) as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to insure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items shall meet all requirements of sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of ensuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling inspection, as part of manufacturing operations, is an acceptable practice to ascertain conformance to requirements, however, this does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to accept defective material.

4.2 Classification of inspections. The inspection requirements specified herein are classified as follows:

a. First article inspection (see 4.4)

b. Quality conformance inspection (4.5)

4.3 Inspection conditions. Unless otherwise specified, all tests required by this specification shall be made at an atmospheric pressure of 28 to 32 inches of mercury, at a temperature of 77°$\pm$18°F, and at a relative humidity of 80 % or less. Where tests are conducted with atmospheric pressure or temperature substantially different from these values, proper allowance shall be made for the change in instrument reading.

4.4 First article inspection. First article inspection shall consist of all the examinations and tests specified (see 4.6).

4.4.1 Samples. The first article inspection shall be performed on one dummy converter which is representative of the construction, workmanship, components, and materials to be used during production. When a contractor is in continuous production from contract to contract, submission of further first article samples or test reports may be waived at the discretion of he procuring activity. Approval of the first article inspection or the waiving of the first article inspection does not preclude the requirements of performing the quality conformance inspection.

4.4.2 Manufacturer's inspection report. When specified by the procuring activity a test report prepared in accordance with MIL-STD-831, shall include the results of all tests including a detailed statement indicating compliance or extent of noncompliance with each requirement of this specification. The report shall be forwarded to the procuring activity together with the tested samples unless otherwise specified (see 6.3).

4.4.3 Accept-reject criteria for reliability testing. The accept-reject criteria for reliability testing of the first articles shall be in accordance with MIL-STD-781, Test Plan I.

4.5 Quality conformance inspections. Quality conformance inspections shall consist of:

a. Individual inspections.(see 4.5.1).

b. Sampling inspections.(see 4.5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

4.5.1 Individual inspections. Each dummy converter on the contract or order shall be subjected to the following examination and tests. Any dummy converter containing a defect shall be rejected.

a. Examination of product (see 4.6.1).

b. Capacitance at room temperature (see 4.6.2).

4.5.2 Sample inspection. Two dummy converters shall be selected at random from each lot of 200 or fraction thereof and subjected to the following tests as described under 4.6:

a. Capacitance at low temperature (see 4.6.3).

b. Capacitance at high temperature (see 4.6.4).

c. Immersion (leakage) (see 4.6.5).

4.5.2.1 Rejection and retest. If one or more items from a lot fail to meet the specification, acceptance of all items in the lot shall be withheld until the extent and cause of the failure have been determined. The contractor shall explain fully to the Government representative the cause of the failure and the action taken to preclude recurrence. After correction, all of the sampling tests shall be repeated.

4.6 Test methods

4.6.1 Examination of product. Each dummy converter shall be carefully examined to determine conformance to the requirements of this specification with respect to material, design, construction, weight, marking, and workmanship.

4.6.2 Capacitance at room temperature. The capacitance shall be determined at room temperature by using a master test instrument of suitable accuracy. The capacitance shall be as specified (see 3.5.1).

4.6.3 Capacitance at low temperature. The dummy converter shall be cold soaked at -65°F for at least 8 hours. While still at this temperature, the capacitance shall be determined with a suitable master test instrument. The capacitance shall be as specified (see 3.5.2).

4.6.4 Capacitance at high temperature. The dummy converter shall be maintained at a temperature of at least plus 260°F for at least 8 hours. While still at this temperature, the capacitance shall be determined with a suitable master test instrument. The capacitance shall be as specified (see 3.5.3).

4.6.5 Immersion (leakage). The dummy converter shall be subjected to the immersion (leakage) test specified in accordance with MIL-STD-810, method 512, procedure I. The leakage shall be as specified (see 3.5.4).

4.6.6 Reliability test level. The reliability test level shall consist of temperature and vibration cycling as follows: The dummy converter shall be stabilized at a temperature of -65°F, then stabilized at a temperature of 260°F and held for at least two hours, then returned to a temperature of -65°F. The transition period in changing between temperature extremes shall not exceed 40 minutes. The dummy converter shall be subjected to at least four of these temperature cycles per 24 hours. The dummy converter shall be subjected to vibration at any frequency between 20 and 60 cycles per second and an applied acceleration of $\pm$2g for at least 10 minutes within each hour of this test. Rated voltage $\pm$2% shall be applied continuously during this test. A failure shall be identified as any malfunction which causes excessive error in the capacitance value of the dummy converter. The dummy converter shall be checked at least once every 24 hours at each temperature extreme to determine if a failure has occurred. No parts shall be replaced as preventive maintenance during reliability testing (see 3.5.5).

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

4.6.7 Maintainability verification. Time studies of all corrective maintenance tasks for all expected failure modes shall be conducted by simulating failures. Timing of each maintenance task shall be performed at least three times to determine average values. The maintenance tasks considered shall be only those related to field level maintenance. The time to accomplish each maintenance task shall include time for preparation, recognition, fault location, removal (based only on the installation provisions of the item), fault correction, adjustment and realignment, final test, and replacement, but shall exclude supply time and administrative time. In the case of repetitive subtasks which occur by the nature of the sequence of maintenance actions (e.g., removal), it shall not be necessary to redetermine the average time required.

4.7 Inspection of packaging. Except when commercial packaging is specified, the sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification shown in section 5. The inspection of marking for shipment and storage shall be in accordance with MIL-STD-129. The inspection of commercial packaging shall be as specified in the contract (see 6.2).

5. PACKAGING.

5.1 Preservation. Preservation shall be level A as specified (see 6.2).

5.1.1 Level A.

5.1.2 Cleaning. Cleaning shall be in accordance with Air Force Drawing 8148650.

5.1.3 Drying. Drying shall be in accordance with Air Force Drawing 8148650.

5.1.4 Preservative application. Preservatives shall not be used.

5.1.5 Unit pack. Unless otherwise specified by the procuring activity, items shall be packaged in Quantity Unit Pack (QUP) of one each. Preservation for each item shall conform to MIL-P-116, submethod IA-8.

5.2 Packing. Packing shall be level "A", "B", or "C", as specified (see 6.2).

5.2.1 Container-cushioning. Unit container requirements shall conform to MIL-B-131, barrier material, unless otherwise specified by the procuring activity. Unit containers shall be large enough to allow for application of sufficient wrap (MIL-B-121) material, and cushioning material, between the item and unit container. Item cushioning/wrap material shall conform to PPP-C-1797 and provide sufficient density and thickness to protect the unit container from punctures. Intermediate and/or shipping container requirements shall conform to ASTM D5118/D5118M, (see 6.2.1.2) Regular Slotted (RSC/0201) as specified by the procuring activity. Cushioning material shall be of sufficient density and thickness to insure shock transmission does not exceed peak values which have been established for the item.

5.2.2 Level A. Dummy converters, preserved as specified (see 5.1) shall be packed in containers in accordance with PPP-B-601.

5.2.3 Level B. Dummy converters , preserved as specified (see 5.1) shall be packed in exterior containers in accordance with ASTM D5118/D5118M Type weather-resistant unless otherwise specified by the contracting activity. Exterior container shall be uniform shape, size and minimum tare and cube, consistent with the protection required. Closure shall be in accordance with ASTM D1974, Sealing Method A procedures or as specified by contracting activity.

5.2.4 Level C. Dummy converters, preserved as specified (see 5.1) shall be packed in such a manner that will afford adequate protection against physical/mechanical damage during direct domestic shipment from the supply source to the first receiving activity. These containers shall be in accordance with ASTM D5118/D5118M.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

5.3 Marking. All unit and shipping containers shall be marked in accordance with MIL-STD-129. In addition, the following precautionary marking shall appear on the unit and shipping container:

Oxygen Components - All oil, grease,
shop residue, or other contaminants
have been removed.

Do not open until ready for use.

6. NOTES

(This section contains information of a general or explanatory nature that may be helpful, but is not mandatory.)

6.1 Intended use. The dummy converters covered by this specification are intended to be used in F-111, F-14, F-15 and B52 aircraft when one of the converters is not installed.

6.2 Acquisition requirements. Acquisition documents must specify the following:

a. Title, number, and date of this specification.

b. Issue of DODISS to be cited in the solicitation, and if required, the specific issue of individual documents referenced (see 2.1).

c. Type of dummy converter (see 1.2 and 6.6)

d. Selection of applicable levels of preservation, packaging, and packing (see 5.1 and 5.2).

e. Items of data required (see 6.3).

6.3 Consideration of data requirements. The following data requirements should be considered when this specification is applied on a contract. The applicable Data Item Descriptions (DID's) Should be reviewed in conjunction with the specific acquisition to ensure that only essential data are requested/provided and that the DID's are tailored to reflect the requirements of the specific acquisition. To ensure correct contractual application of the data requirements, a Contract Data Requirements List (DD Form 1423) must be prepared to obtain the data, except where DOD FAR Supplement 27.475-1 exempts the requirement for a DD Form 1423.

Reference Paragraph	DID Number	DID Title
4.4.2	DI-NDTI-80809A	Test / Inspection Report

The above DID's were cleared as of the date of this specification. The current issue of DOD 5010.12-L, Acquisition Management Systems and Data Requirements Control List (AMSDL), must be researched to ensure that only current, cleared DID's are cited on the DD Form 1423.

6.4 First article. When first article inspection is required, the contracting officer should provide specific guidance to offerors whether the item should be a preproduction sample, a first article sample, a first production item, a sample selected from the first production items, a standard production item from the contractor's current inventory (see 3.1), and the number of items to be tested as specified (see 4.4.1). The contracting officer should also include specific instructions in acquisition documents regarding arrangements for examinations, approval of first article test results, and disposition of first articles. Invitations for bids should provide that the Government reserves the right to waive the requirements for samples for first article inspection to those bidders offering a

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

product which has been previously acquired or tested by the Government, and that bidders offering such products, who wish to rely on such production or test, must furnish evidence with the bid that prior Government approval is presently appropriate for the pending contract. Bidders should not submit alternate bids unless specifically requested to do so in the solicitation.

6.5 Cross reference. This specification supersedes MIL-C-26393. All items that conform to MIL-C-26393 are interchangeable with M26392-2.

6.6 Part or Identifying Number (PIN). The PIN is as follows:


PIN	Type	Designation	Liters
M26392-1	1	CRU-23/A	10
M26392-2	2	CRU-24/A	25

6.7 Subject term (key word) listing:

Breathing oxygen
Capacitance
Capacitor
Case
Interchangeability
Maintainability
Reliability
Simulator
Temperature
Weight

6.8 Changes from previous issue. Marginal notations are not used in this revision to identify changes with respect to the previous issue due to the extensiveness of the changes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

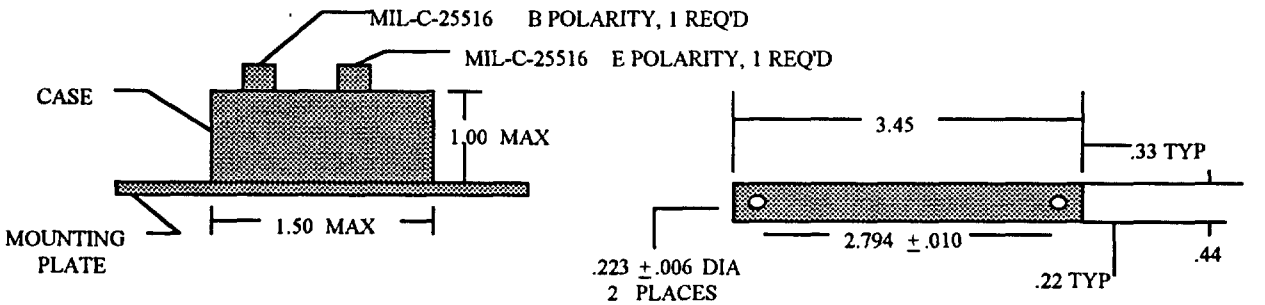


DIMENTIONS IN INCHES
UNLESS OTHERWISE SPECIFIED
TOLERANCES ± .010 FOR .XXX
± .05 FOR .XX

CASE SHALL BE CENTERED ON MOUNTING PLATE

PROTECTIVE COVERS FOR THE CONNECTORS SHALL BE PROVIDED AND SECURED TO THE DUMMY CONVERTER

FIGURE 1 Outline dimensions and mounting plate for type 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

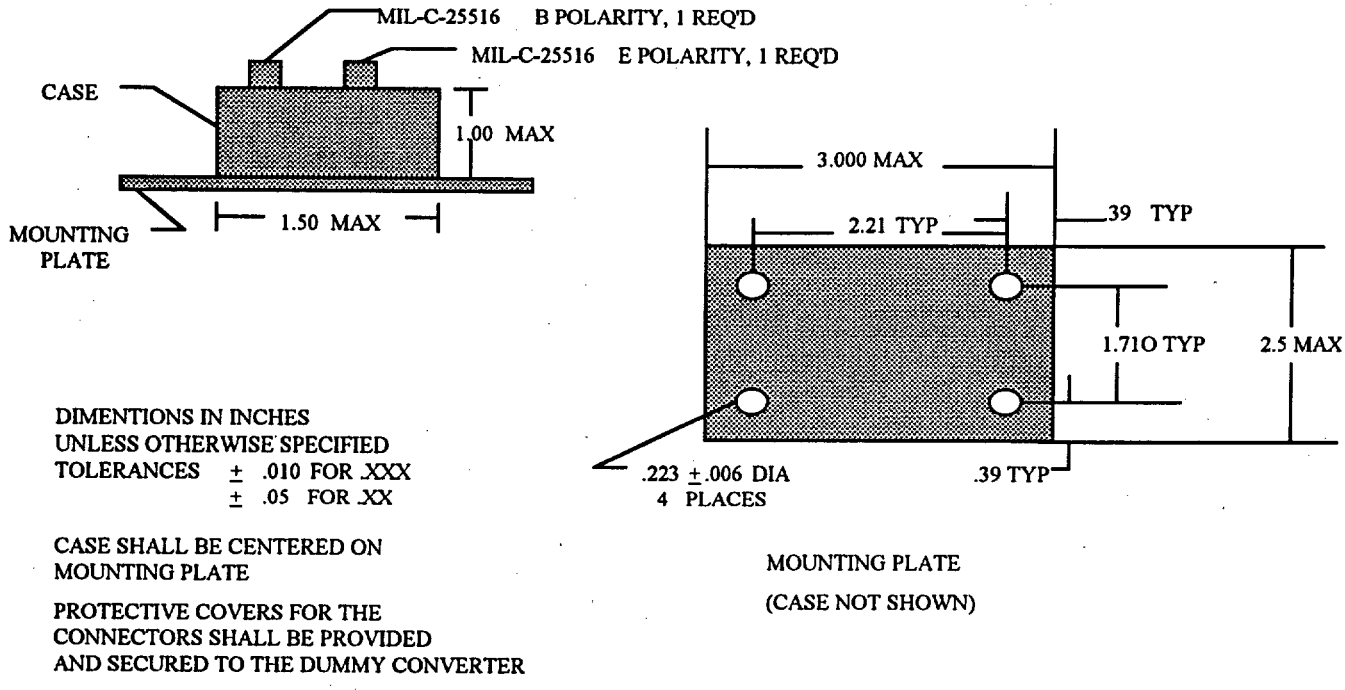

DIMENTIONS IN INCHES
UNLESS OTHERWISE SPECIFIED
TOLERANCES ± .010 FOR .XXX
± .05 FOR .XX

CASE SHALL BE CENTERED ON MOUNTING PLATE

PROTECTIVE COVERS FOR THE CONNECTORS SHALL BE PROVIDED AND SECURED TO THE DUMMY CONVERTER

FIGURE 2. Outline dimensions and mounting plate for type 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

Custodians:
Air Force - 99

Reviewer:
Air Force - 11

Preparing Activity:
Air Force - 71

Agent:
Air Force - 99

(Project 1660-F653)

Source: https://assist.dla.mil -- Downloaded: 2026-10-20T09:33Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	MIL-D-26392C	941028

3. DOCUMENT TITLE

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
OC-ALC/TICLA	405/736-5960	336-5960
c. ADDRESS (Include Zip Code) 3001 Staff Drive Tinker AFB OK 73145-5990	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-20109:332
Check the source to verify that this is the current version before use.