

FED. SUP CLASS
6640

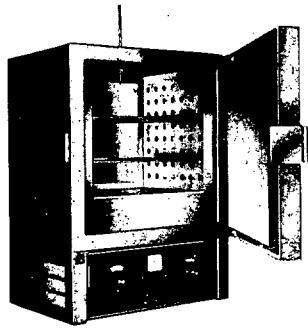

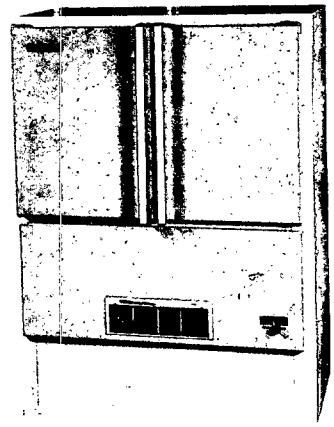

PART NUMBER	NOM INNER CHAMBER CM (IN)			OPERATING TEMP-AMBIENT TO DEG C	WATTS MAX	NO. OF DOORS
	WIDTH	DEPTH	HEIGHT			
BENCH MODELS						
MS36154-1	63 (25)	51 (20)	51 (20)	343	5,200	1
MS36154-2	33 (13)	35 (14)	33 (13)	225	1,150	1
MS36154-3	63 (25)	51 (20)	95 (38)	204	5,500	1
MS36154-4	46 (18)	35 (14)	48 (19)	225	1,420	1
MS36154-5	48 (19)	44 (17.5)	45 (18)	204	2,400	1
MS36154-6	46 (18)	35 (14)	48 (19)	225	1,340	1
MS36154-7	48 (19)	44 (17.5)	45 (18)	204	2,600	1
MS36154-8	48 (19)	44 (17.5)	45 (18)	300	4,500	1
MS36154-9	120 (48)	61 (24)	90 (36)	204	9,800	2
MS36154-10	33 (13)	31 (12)	31 (12)	260	1,000	1
FLOOR MODELS						
MS36154-11	51 (20)	45 (18)	51 (20)	704	10,000	1
MS36154-12	63 (25)	51 (20)	51 (20)	704	13,000	1
MS36154-13	69 (27)	48 (19)	64 (25)	325	6,000	2
MS36154-14	94 (37)	48 (19)	64 (25)	325	6,000	2
MS36154-15	48 (19)	48 (19)	48 (19)	325	4,500	1

MATERIAL: The exterior wall shall be heavy-gauge steel, reinforced at all stress points. Interior shall be heavy gauge solid aluminum, aluminized steel, or stainless steel. The door shall have the same basic construction with swing pivot hinges, magnetic catch and heat resisting handle.

FINISH: The exterior shall be finished with durable baked enamel over a suitable primer coating.

DESIGN: Ovens shall be convection or radiant heat type with a mechanical forced air circulation system. They shall be rectangularly shaped with double walled construction and equipped with two or more shelves, a thermometer, indicator light, variable thermometer, indicator light, variable thermostat control, heater power input switch(es) and heating elements.

Shelves shall be removable, adjustable, and so constructed as to allow proper air circulation throughout the inner chamber.

Oven shall have an adjustable air flow system that permits the air to

APPROVED 13 OCT 1983 REVISED

USER ACTIVITIES: ARMY - DM, MD
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - AS, YD
AIR FORCE - 82

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A. EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust MS 99		OVEN, LABORATORY, FORCED AIR, MECHANICAL CONVECTION	MS36154
Procurement Specifications NONE	SUPERSEDES:		SHEET 1 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1206

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:35Z
Check the source to verify that this is the current version before use.

pass horizontally through the chamber only once when necessary and to allow almost 100% exhaust of fumes. Exhaust shall have damper control.

Insulation shall be a minimum of 76 mm thick and shall completely envelop the inner chamber of the oven, including the door.

Ovens with two doors shall have no center mullion.

Ovens shall be in accordance with the requirements as specified in ASTM E145.

Heating unit shall operate at 120/240 volts, 50/60 Hz, single phase, as specified at invitations for bid.

All electrical components and insulations shall conform to the standards of Underwriters Laboratories, Incorporated.

NOTES:

1. Overall dimensional limitations and color of exterior shall be specified on date of invitations for bid.

2. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

3. Referenced documents shall be of the issue in effect on date of invitations for bid.

4. FSCM: 15486, 48619, and 95632.

USER ACTIVITIES:

REVIEWER ACTIVITIES:

APPROVED

REVISED

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A. EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust MS 99		OVEN, LABORATORY, FORCED AIR, MECHANICAL CONVECTION	MS36154
Procurement Specifications NONE	SUPERSEDES:		SHEET 2 OF 2

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE

PROJECT NUMBER 6640-1206

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:35Z
Check the source to verify that this is the current version before use.