00-G-00684b(DSA-DM)
15 March 1967
Revision of 00-G-684
31 July 1958
Superseding 00-G-00684a(DM)
3 February 1964

INTERIM FEDERAL SPECIFICATION

GRINDING AND POLISHING MACHINE, DENTAL LABORATORY, Floor Mounted, 110 Volt, 60 Cycle, A.C.

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania, 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification 00-G-684.

1. SCOPE

1.1 Scope. This specification covers a floor mounted dental laboratory grinding and polishing machine, suitable for operation on 115 volt, 60 cycle, alternating current.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

CC-M-636	Motor, Alternating-Current (Fractional-Horsepower).
NN-P-530	Plywood; Flat Panel.
QQ-A-250/2b	Aluminum Alloy 3003, Plate and Sheet.
UU-P-271	Paper, Wrapping, Waterproofed Kraft.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.

STANDARDS

Federal

FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D.C., 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

(Copies of Military specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:00Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

UNDERWRITERS' LABORATORIES, INC.

Underwriters' Laboratories Standards:

UL73 - Standard for Motor Operated Appliances.
UL496 - Standard for Edison-Base Lampholders.

(Underwriters' Laboratories Standards are available from the Underwriters' Laboratories, Inc., Walt Whitman Road, Melville, L.I., N.Y., 11749, 207 E. Ohio Street, Chicago, Illinois, 60611, and 1655 Scott Blvd., Santa Clara, Calif., 95050.)

UNITED STATES OF AMERICA STANDARDS INSTITUTE *

USA C73.11-1963 USA Standard for Outlet Receptacles, Attachment Plug Caps and Appliance Plugs.

(Application for copies should be addresed to The United States of America Standards Institute, 10 East 40th Street, New York, N.Y. 10016.)

* Formerly the American Standards Association. All ASA Standards are now designated as USA Standards.

3. REQUIREMENTS

3.1 First Article. Unless otherwise specified, prior to the start of production of the contract quantity, one sample of the grinding and polishing machine shall be assembled, completely finished, and tested by the contractor. The sample shall be submitted, together with the contractor's inspection and test reports, to the procuring contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the procuring contracting officer, or his authorized representative, prior to the manufacture and assembly of the remaining quantity to be manufactured. Pending approval of the first article, acquisition of materials, components, or commencement of production is at the sole risk of the contractor. Accepted sample shall become the property of the procuring activity and shall be included in the quantity called for in the contract or order. In the event that the sample is not approved, the contractor shall submit a new sample for approval, or modify the existent sample so as to remove the deficiencies cited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the current version before use.

3.2 Fire and casualty hazards.

3.2.1 The contractor shall submit proof to the contracting agency, prior to delivery, that the equipment he will supply under this specification conforms to the applicable requirements of Underwriters' Laboratories, Inc. Standards UL73 and UL496. The label or listing of the Underwriters' Laboratories, Inc. may be accepted as evidence that the equipment conforms to this requirement.

3.2.2 In lieu of the label or listing, the contractor may submit independent proof satisfactory to the contracting agency, prior to delivery, that his equipment conforms to the Underwriters' Laboratories, Inc. Standards.

3.2.3 Compliance with Underwriters' Laboratories, Inc. requirements regarding fire and casualty hazards does not absolve the contractor from complete compliance with the requirements of this specification in order to secure the acceptance of his commodity.

3.3 Materials. Materials shall conform in all respects to the specifications listed in section 2, and as hereinafter specified. When materials are used which are not specifically designated, they shall be of high commercial quality throughout, and suitable in all respects for the purpose intended. The materials in all cases shall be consistent with the strength required for safety and durability.

3.3.1 Sheet aluminum. The sheet aluminum shall be alloy 3003, in conformance with QQ-A-250/2b for H14 temper. Thickness of sheet shall be a minimum of 0.032 inch (20 Brown and Sharpe) (B&S) gage.

3.3.2 Plywood. The plywood shall be 5-ply, either Douglas fir, interior type, grade A-D, or hardwood, medium density, type II, grade 2, in conformance with NN-P-530.

3.3.3 Wire cloth. The wire cloth used in the fabrication of the screen specified in 3.5.10 shall be galvanized steel wire, 4 by 4 mesh size, and the wire diameter shall be 0.035 plus or minus 0.003 inch in diameter.

3.4 Style, design and construction. Style, design and construction of the grinding and polishing machine shall be as shown in Figure 1. Machines shall be suitable for grinding and polishing operations and for filtering grinding debris in dental prosthetic procedures. The component parts of the machine shall be properly aligned prior to welding and riveting into permanent position, so as to provide a straight, rigid, durable construction and level working assembly.

3.5 Components. The grinding and polishing machine shall consist essentially of a cabinet with a removable front panel, tabletop, hoods, splash pans, work shelf, blower unit, polishing lathe, filters, tray, screen, and accessories as hereinafter specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:00Z
Check the source to verify that this is the current version before use.

3.5.1 Cabinet. The sides, back, bottom, and removable front panel of the cabinet shall be fabricated of sheet aluminum alloy as specified in 3.3.1, with all parts securely welded, except as an alternate, interior aluminum shell parts shall be securely riveted or bolted, or as an alternate, both riveted and bolted to the sides of the cabinet. The sides, back, and bottom shall be riveted to an angle iron framework. The vertical framework forming the four corners, shall extend below the bottom of the cabinet, serving as legs. Right angle footings shall be securely fastened to the ends of the legs by welds, rivets, bolts, or other suitable means. A set of four rubber caster cups shall be furnished for placement on footings in order to cushion the machine. The front panel of the cabinet shall be equipped with suitable means for easy removal, without the use of tools. The outside measurements of the cabinet shall be 28-1/2 plus or minus 1/2 inches in width, 17 plus or minus 1 inches in depth, and 38 plus or minus 1/2 inches in height, when measured from the floor to the working surface of the tabletop.

3.5.2 Tabletop. Tabletop shall be made of 5/8-inch plywood as specified in 3.3.2, bounded on sides and back with a solid wood railing, and covered on top with sheet aluminum as specified in 3.3.1 The railing shall be 1-3/4 inches high and 3/4 inches thick. The working surface of the tabletop shall be 29-1/2 plus or minus 1/2 inches wide and 17-1/2 plus or minus 1/2 inches deep.

3.5.3 Hoods and splash pans. Hoods and splash pans shall be fabricated of sheet aluminum as specified in 3.3.1. Hoods shall be 13 plus or minus 1/2 inches high, 7-1/8 plus or minus 1/8 inches wide, and 10 inches deep, and shall be screwed to the tabletop. Each hood shall be equipped with a standard lampholder. Splash pans shall be separate from the hoods for convenient removal and cleaning, and suitable means shall be provided for holding the pans securely in place. One pan shall have an aluminum wire screen welded to back section, which shall extend 6-1/4 inches above top of pan, and shall be bent forward at an angle of 15 degrees. The other pan shall have a solid aluminum sheet, as specified in 3.3.1, welded to back section, which shall extend 3-5/8 inches above top of pan, and shall be bent forward at an angle of 30 degrees. Splash pans shall be 7 inches wide, 2 inches high, and 10-1/2 inches long, including angulated front. The pans shall extend frontally 3-1/2 $\pm$ 1/2 inches at the bottom and 5-1/2 $\pm$ 1/2 inches at the top from front edges of the hood. All edges and corners of the hood and splash pans shall be rounded, ground smooth, or otherwise treated to eliminate burrs and sharp or ragged edges. Seams shall be spot-welded and a suitable sealant shall be applied on all inside corner seams.

3.5.3.1 Shields. Each hood shall be equipped with a rigid, shatterproof, plastic shield of optical quality, 6 $\pm$ 1/4 inches wide, 9 $\pm$ 1/4 inches long, and 1/8 $\pm$ 1/32 inch thick. The shield shall be securely hinged to the top of the hood and shall be adjustable to the desired visual angle or position. The shield shall be so mounted as to permit its raising to rest on top of the hood, when not in use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:00Z
Check the source to verify that this is the current version before use.

3.5.3.2 Lampholders. A lampholder, or electric bulb socket base, shall be mounted on the upper inside surface of each hood. The lampholder shall be held in a plated steel ring having a minimum of two full threads, and shall be secured to the inside surface of the hood by two screws and nuts. Each lampholder shall be rated at 660 watts, 250 volts, with a type SJ, two-conductor, Number (No.) 18 American wire gage (Awg.) supply cord. The supply cord from each lampholder shall pass through the tabletop, by means of an access hole and rubber grommet insert, and shall terminate within the enclosure of the duplex receptacle. Each lampholder assembly shall have a separate "on-off" switch. The electric bulb shall be adequately protected from debris by a suitable shield. The lampholder assembly shall meet the requirements of applicable Underwriters' Laboratories Standards.

3.5.4 Work shelf. Work shelf shall be made of 5/8 inch plywood as specified in 3.3.2, and shall consist of the working surface covered on top with sheet aluminum, as specified in 3.3.1, except that the sheet thickness shall be 0.025 inches and shall contain a railing 5/8 ± 1/8 inch high nailed to top and surrounding the front and sides. Work shelf shall be supported by two iron rods, securely attached to the tabletop and the under surface of the shelf. Shelf shall be 30-1/2 inches wide and 8-1/2 inches in length, and shall be bent forward at an angle of 15 degrees. Height of shelf above tabletop shall be 17-3/8 inches.

3.5.5 Blower unit. Blower unit shall consist of a unit assembly of blower motor, blower wheel, and blower housing in accordance with 3.5.5.1, 3.5.5.2, and 3.5.5.3, mounted on a spring chassis to eliminate vibration. Spring chassis shall be securely bolted to the framework of the cabinet. Unit shall have a minimum free air capacity of 500 cubic feet per minute (c.f.m.) when driven by a 1/4 horsepower (HP) motor at 1725 revolutions per minute (r.p.m.), venting to the atmosphere.

3.5.5.1 Blower motor. Blower motor shall conform to the applicable requirements of CC-M-636 for type I, class 1a, style A-1 and A-2, continuous duty. Motor furnished shall be split-phase, squirrel cage, capacitor-start, rated 1/4 HP, 1725 r.p.m., single-phase, 115/230 volts, 4.6/2.3 amperes, 60 cycle, 40 degrees centigrade (°C.) temperature rise, J56 Frame, Service Factor (SF) 1.35 inches.

3.5.5.2 Blower wheel. The blower impeller, or wheel, shall be fabricated of aluminum, and shall have an outside diameter of 7-7/8 plus 1/64, minus 3/64 inches, and shall be 3-7/8 plus or minus 1/32 inches wide. The impeller shall be provided with 40 vanes, each 9/16 plus or minus 1/32 inches wide and 3-1/4 plus or minus 1/32 inches long. The blower impeller shall be secured to the motor shaft with key and set screw.

3.5.5.3 Blower housing. The blower housing shall be made of sheet steel 0.045 inch thick (No. 17 B&S Gage). The outside diameter shall be 11-1/8 plus or minus 1/16 inches, with an air inlet diameter of 8-1/32 plus or minus 1/32 inches and rectangular air outlet of 4-13/16 by 5-1/16 inches plus or minus 1/16 inch.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the current version before use.

3.5.6 Polishing lathe. The motor shall conform to the applicable requirements of CC-M-636 for type I, class 1b, style B-1, suitable for intermittent duty, load, no-load, and rest. Motor furnished shall be split-phase, ball bearing type rated 1/4 to 1/6 HP at operating speeds of 1725 r.p.m. and 3450 r.p.m., 116 Frame, 115 volts, 60 cycle, single-phase. The height from bench top to center of shaft shall be approximately 6 inches. The overall length measuring from the extreme end of one shaft to the other shall be 15 plus or minus 1/8 inches, and with two No. 7 chucks mounted, it shall measure 21 plus or minus 1/4 inches. Polishing lathe shall be securely bolted to the bench top.

3.5.6.1 Shaft. The shaft shall be hardened steel alloy, extending at each end of the motor and shall accommodate the standard lathe chucks specified in 3.5.12. The shaft shall be accurately ground to precision limits, and shall be provided with tapered ends for the reception of chucks. The exposed length of shaft, beginning from end of chuck remover, shall be 7/8 plus or minus 1/16 inch. The 1/2 inch diameter shaft shall taper 0.204 inch per foot and end with a shaft diameter of 0.355 plus or minus 0.001 inch at the extreme ends (chuck end attachment). The shaft shall not move parallel to its long axis, except when chucks are being removed.

3.5.6.2 Chuck removing device. A suitable chuck removing device shall be located at each end of the shaft to provide easy removal of chuck by turning of lever handle. The chuck removing device must be designed so that its operation does not exert excess thrust (or chuck load) between the balls and races of the bearing.

3.5.6.3 Control switch. The control switch shall be located in the front of the motor or in the base, and shall be a three position, snap action toggle or lever type. Adequate designation of switch position shall be provided for 'off', 'high speed', and 'low speed' positions.

3.5.7 Connecting cord. Connecting cord for motors shall consist of a rubber covered service cable with a steel armored connector plug attached. The power cords for the lathe and blower motor shall be 3-conductor cables equipped with a 3-prong plug suitable for use with receptacles specified in United States of America Standards Institute (USA) Standard, USA C73.11-1963, for Caps and Receptacles, 125 Volts, 15 Ampere, 2-Pole, 3-Wire Grounding Type. The current rating of the cords shall be not less than that of the motor. External connecting cord shall be not less than 8 feet in length.

3.5.7.1 Switches. All switches shall be totally enclosed, and rigidly mounted to prevent rotation. Where exposed terminals exist, they shall be suitably recessed or provided with a removable guard to prevent shorting of wires or injury to personnel.

3.5.7.2 Equipment wiring. Equipment wiring shall be suitably routed and fastened mechanically. Wire splices shall be totally enclosed and suitably fastened and insulated. All wire terminations shall be strain relieved.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the currentversion before use.

3.5.8 Filters. Two fiber-glass filters shall be positioned 10 inches above the bottom of the cabinet. Each filter shall measure 25 inches wide, 14 plus or minus 2 inches long, and 2 inches thick. Filters shall be easily removable for cleaning.

3.5.9 Tray. A removable tray shall be located at the bottom of the cabinet. Tray shall be 1-1/4 inches high and of sufficient length and width to accommodate the filters specified in 3.5.8. Tray shall be fabricated of sheet aluminum as specified in 3.3.1.

3.5.10 Screen. A galvanized-steel wire screen as specified in 3.3.3, shall be located directly below the lower filter.

3.5.11 Tolerances. Commercial tolerances shall apply for gage size or thickness of material. Unless otherwise specified, a plus or minus tolerance of 1/4 inch shall apply for straight measurements, and plus or minus 3 degrees for angular measurements.

3.5.12 Accessories. Four No. 7 steel taper chucks, suitable for accurate fitting to shaft specified in 3.5.6.1, shall be supplied with each unit, two right and two left. The overall length of chucks shall be 3-5/8 plus or minus 1/8 inches and the threaded portion shall be 2-1/8 inches.

3.6 Finish. The framework of the work shelf shall be suitably finished with a durable green paint flecked with white and black. The blower housing shall be finished with green paint. The supports for the work shelf shall be finished with aluminum paint. All other aluminum sheet paneling shall have a polished finish. All welds shall be accomplished in accordance with standard industrial practice. All exposed welds shall be wire-brushed smooth to eliminate traces of pitmarks, and seams, and shall be polished to blend with adjacent surfaces.

3.7 Identification marking. Each lathe shall have a corrosion-resistant metal nameplate permanently affixed thereto. The plate shall bear the model or style designation, serial number, current, voltage, cycle, and name or registered trademark of the manufacturer. In addition, a second corrosion-resistant metal nameplate shall be permanently affixed to the outside of the removable front panel of the unit, and shall bear the stock number, item identification and contract or purchase order number. The markings on the plates shall be clear and permanent, and shall be accomplished by die stamping into the surface of the metal.

3.8 Service data. The contractor shall furnish, with each unit,two copies of a service data manual. In addition, the contractor shall mail 15 copies of the approved service data to the contracting officer for distribution. This service data shall contain complete instructions for installation, operation, maintenance, and a list of component parts. The service data shall include such detailed information which shall permit ready installation and maintenance of the item. All information contained in the manual shall be suitably indexed to permit ready reference to the required information. Wiring diagrams shall be included for electrical items or components. Wiring diagrams, drawings and descriptive material shall include adequate information so that the replacement parts can be

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the current version before use.

ordered by the manufacturer's part number, and without confusion as to the item identification. Identical or interchangeable replacement parts shall be identified by a single part number only. One set of the service data, as indicated above, shall be placed in a sealed, waterproof envelope, and affixed securely to the outside of the exterior container. The envelope shall be secured to the exterior container by use of metal ties, nails, or similar means, and shall be located at the end of the exterior container, preferably, when space permits, at the end bearing the markings required by MIL-STD-129. In cases where complete service data is too bulky to be conveniently attached to the outside of the exterior container, the contents of the exterior envelope may be limited to information necessary for roughing-in preparations, and a note shall be made on the exterior envelope which shall indicate where the remainder of the first set of service data will be located. The envelope shall be affixed to the container designated as No. 1 of the set. The second set, and, if necessary, the remainder of the first set of service data shall be attached to the unit inside the exterior container.

3.8.1 Approval of Service Data. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the contracting officer, via the cognizant Government inspector, two preliminary copies of his proposed service data, for review and comment by Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary service data shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of required revisions and corrections in the final service data without delaying delivery under the contract or purchase order.

3.8.2 Waiver of Review and Distribution Copies of Manual. Should the supplier have furnished manuals which have been reviewed, commented on, and approved by the Directorate of Medical Materiel for the identical item within two years preceding the date of contract, and propose to furnish manuals identical with those previously approved, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request.

3.9 Workmanship. Workmanship shall be first class throughout. The grinding and polishing machine shall be free from defects which detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.4.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the currentversion before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The Inspection Level and Acceptable Quality Level (AQL) shall be as indicated in Table I.

Table I. Inspection and Acceptable Quality Levels

Type Defect	Inspection Level	Acceptable Quality Level (percent defective)
Major	II	1.0
Minor	II	2.5
Minor A	S2	4.0

4.2.2 For testing. Each grinding and polishing machine shall be given an operational test as specified in 4.4.1. Any failure shall be sufficient cause for rejection.

4.3 Examination. Grinding and polishing machines shall be examined for defects including, but not limited to, those listed in Table II.

Table II. Classification of Defects

Categories	Defects
Critical:	None defined
Major:	
101	Weld missing or not complete.
102	Machine components not properly assembled.
103	Machine framework not square and level.
104	Sharp edges,burrs, and slivers present on hood and splash pans.
105	Rivets improperly set, loose, or missing.
106	Any component missing.
Minor:	
201	Shields have blemished and scratched surface.
202	Exposed surfaces not free from rough edges.
203	Welds not ground or polished to blend into adjacent surfaces.
204	Finish not as specified.
205	Units not free of dirt, oil, or grease.
206	Identification marking missing, incomplete, or illegible.
Minor A:	
250	Wire cloth not correct mesh size.
251	Wire cloth and sheet aluminum thickness not as specified.
252	Frame and work shelf dimensions not as specified.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the currentversion before use.

4.4 Tests.

4.4.1 Operational test. Each polishing lathe and blower unit shall be started and stopped to insure that it is functioning properly without undue noise, vibration and abnormal speed. The polishing lathe shall be operated at the high and low speed levels by proper starting switch procedures. The blower unit shall be tested to insure that adequate forced air is available for the safe disposal of dust and grit.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One grinding and polishing machine, as specified, constitutes one unit.

5.1.2 Level A.

5.1.2.1 Unit preparation. Each unit shall be disassembled as far as is practicable. Surfaces subject to corrosion shall be cleaned and treated with a suitable rust preventive. All exterior finished surfaces shall be protected by wrapping with kraft paper and cushioning with flexible corrugated fiberboard or other suitable materials. Wrapping and cushioning material shall be secured by tying with cotton cord or tape, or by sealing with kraft gummed paper tape. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit.

5.1.3 Level C. Unit shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 Level A. Each unit shall be overpacked in an exterior container designed for type 3 load, and constructed in accordance with PPP-B-601, table II, using type III, class 1 plywood or PPP-B-621, table IV. Closure and strapping shall comply with appendix of applicable specification. Each box shall be lined with a waterproof barrier fabricated of material conforming to UU-P-271 and sealed with suitable waterproof adhesive. The exterior container design shall include three skids of not less than 1-1/2 inches in thickness applied crosswise of base, so positioned as to facilitate handling with a forklift truck, and to maintain unit in an upright position. The unit shall be adequately secured within the exterior container by means of bolts, wood braces, blocks or other suitable devices, to insure against shifting and breaking, or marring of surfaces.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the currentversion before use.

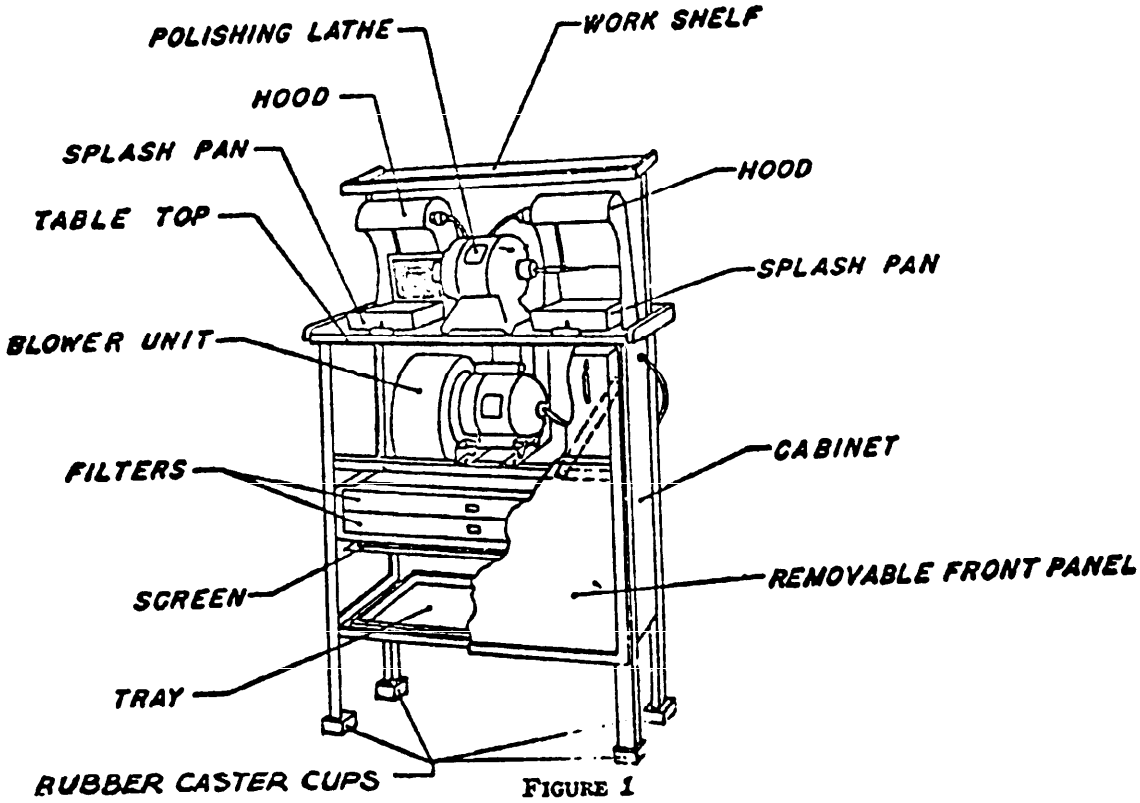


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
AUG 66

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:00Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION

00-G-00684b(DSA-DM)

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1 JAN 66 1426

REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:00Z
Check the source to verify that this is the current version before use.