
2-1212

FED. SUP CLASS
6630

REVIEW ACTIVITIES: ARMY - WC, MI, ME

USER ACTIVITIES: ARMY - EL

This military standard is approved by the Department of Defense and is mandatory on all activities. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

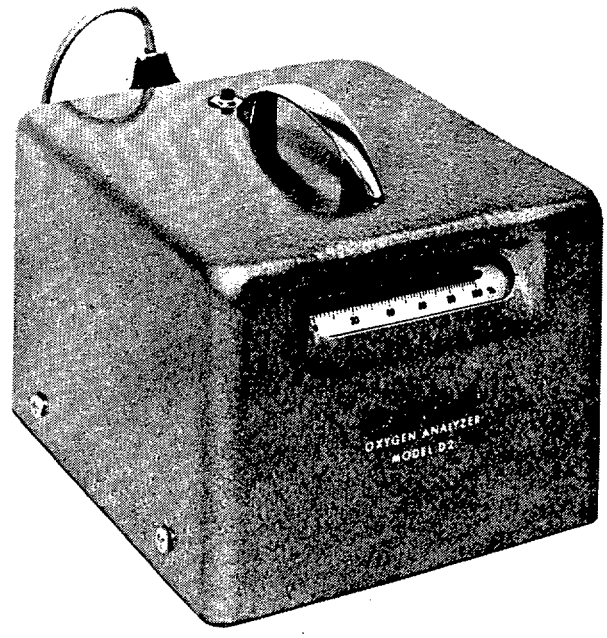

PART NUMBER	O/A DIMENSIONS (in.)			ANALYTICAL PERCENT RANGE	PARTIAL PRESSURE RANGE	PERCENT READING ACCURACY	ANALYSIS CELL VOLUME
	D	W	H				
MS36524-1	7	6	5	0 to 100	0 to 760 mm	± 2	10 ml

MATERIAL: Dumbbell shall be of glass.

Suspension line shall be of quartz fiber.

Case shall be of drawn aluminum with gray hammer tone finish.

DESIGN: Analyzer shall be of the type which utilizes the magnetic susceptibility of oxygen. It shall consist of a small dumbbell suspended on a taut fiber in a non-uniform magnetic field which is contained in a corrosion resisting analysis cell. Analyzer shall be battery operated and calibrated to read correctly without adjustment. Gas to be tested shall be free of solids or liquids with temperature near 25°C (77°F).

PURPOSE: For quantitative oxygen determinations of air used in respiratory aids such as oxygen tents and incubators. This item is for static samples only.

NOTE: Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements as specified herein.

APPROVED 29 JUN 1967 REVISED

P.A. MU	TITLE	MILITARY STANDARD
Other Cust MS 82	ANALYZER, OXYGEN (portable, deflection type)	MS36524
Procurement Specification NONE	SUPERSEDES:	SHEET 1 OF 1

DD FORM 1 SEP 68 672 (Continued) EDITION OF 1 SEP 67 MAY BE USED.

U.S. GOVERNMENT PRINTING OFFICE: 1967-301-511/1212

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:42Z
Check the source to verify that this is the current version before use.