A-A-51642
3 September 1986

COMMERCIAL ITEM DESCRIPTION

HOOK, INCUS, HOUSE

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers incus hooks of the House design for use during middle ear microsurgical procedures.

Salient characteristics:

General. The hooks shall be of the House design to use in microsurgical procedures on the middle ear to elevate the incus bone.

Characteristics. Shall be 6-1/2 inches long with a small dull hook at the distal tip. The shank shall have a 15° bend and be sufficiently ductile to allow reshaping by the user. The hook shall be perpendicular to the plane containing the shank and the handle. The right and left instruments are symmetrical to each other, with the shank tapering from the handle to the distal tip. The handle shall be 3-1/2 inches long and 3/16 inches in diameter. The handle shall have a 6 to 8 longitudinal serrations for a more positive grip. The hooks shall be in accordance with Figure 1.

Material. The hooks shall be fabricated from class 4 martensitic stainless steel, shown in Table 2 of ASTM F899. The finished instruments shall comply with the hardness and corrosion testing requirements contained in Federal Specification GG-I-526.

Hardness. When determined in accordance with ASTM E18 or E92, the finished Rockwell hardness of the distal end shall be C50 to C54 and the shank and handle shall have a finished Rockwell hardness of C15 to C20. If the finished Rockwell hardness of the distal end cannot be determined, a Deflection Test shall be used. The distal end shall show no permanent deflection following a bend of 4-1/2 degrees minimum, no more than 3 degrees permanent deflection following a bend of 10 degrees minimum, and no sign of rupture or fracture following a bend of 20 degrees minimum, when tested as specified herein.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:59Z
Check the source to verify that this is the currentversion before use.

Workmanship. The hooks shall be free from defects which detract from their appearance or impair their serviceability.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One hook, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Deflection test. The first 5/32 inch of the distal end of the hook shall be clamped by means of a hemostatic forceps. The tip shall be bent back (away from the handle in the direction the tip would deflect during normal usage) 4-1/2 degrees (minimum) and the measured for permanent deflection after release. The same instrument shall then be subjected to a bend of 10 degrees (minimum) in the same manner and then measured for permanent deflection after release. The same instrument shall then be subjected to a bend of 20 degrees (minimum) in the same manner and then examined for rupture or fracture after release. Examination for rupture or fracture shall be a under a minimum of 30 power (30X) magnification. Test shall be conducted at room temperature.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The unit of product for test purposes shall be one hook. At an inspection level of S-2, the AQL for dimensions shall be 2.5 percent, and corrosion and hardness or deflection testing, 1.0 percent. A minimum of 3 hooks shall be deflection tested per lot.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:59Z
Check the source to verify that this is the currentversion before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8343	HOOK, INCUS, Left, House, 6-1/2 Inch (16.51 cm)
6515-01-139-8344	HOOK, INCUS, Right, House, 6-1/2 Inch (16.51 cm)

Ordering data (Interior/exterior package quantities and labeling and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
DSA-MPQAS

Project No. 6515-3480

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

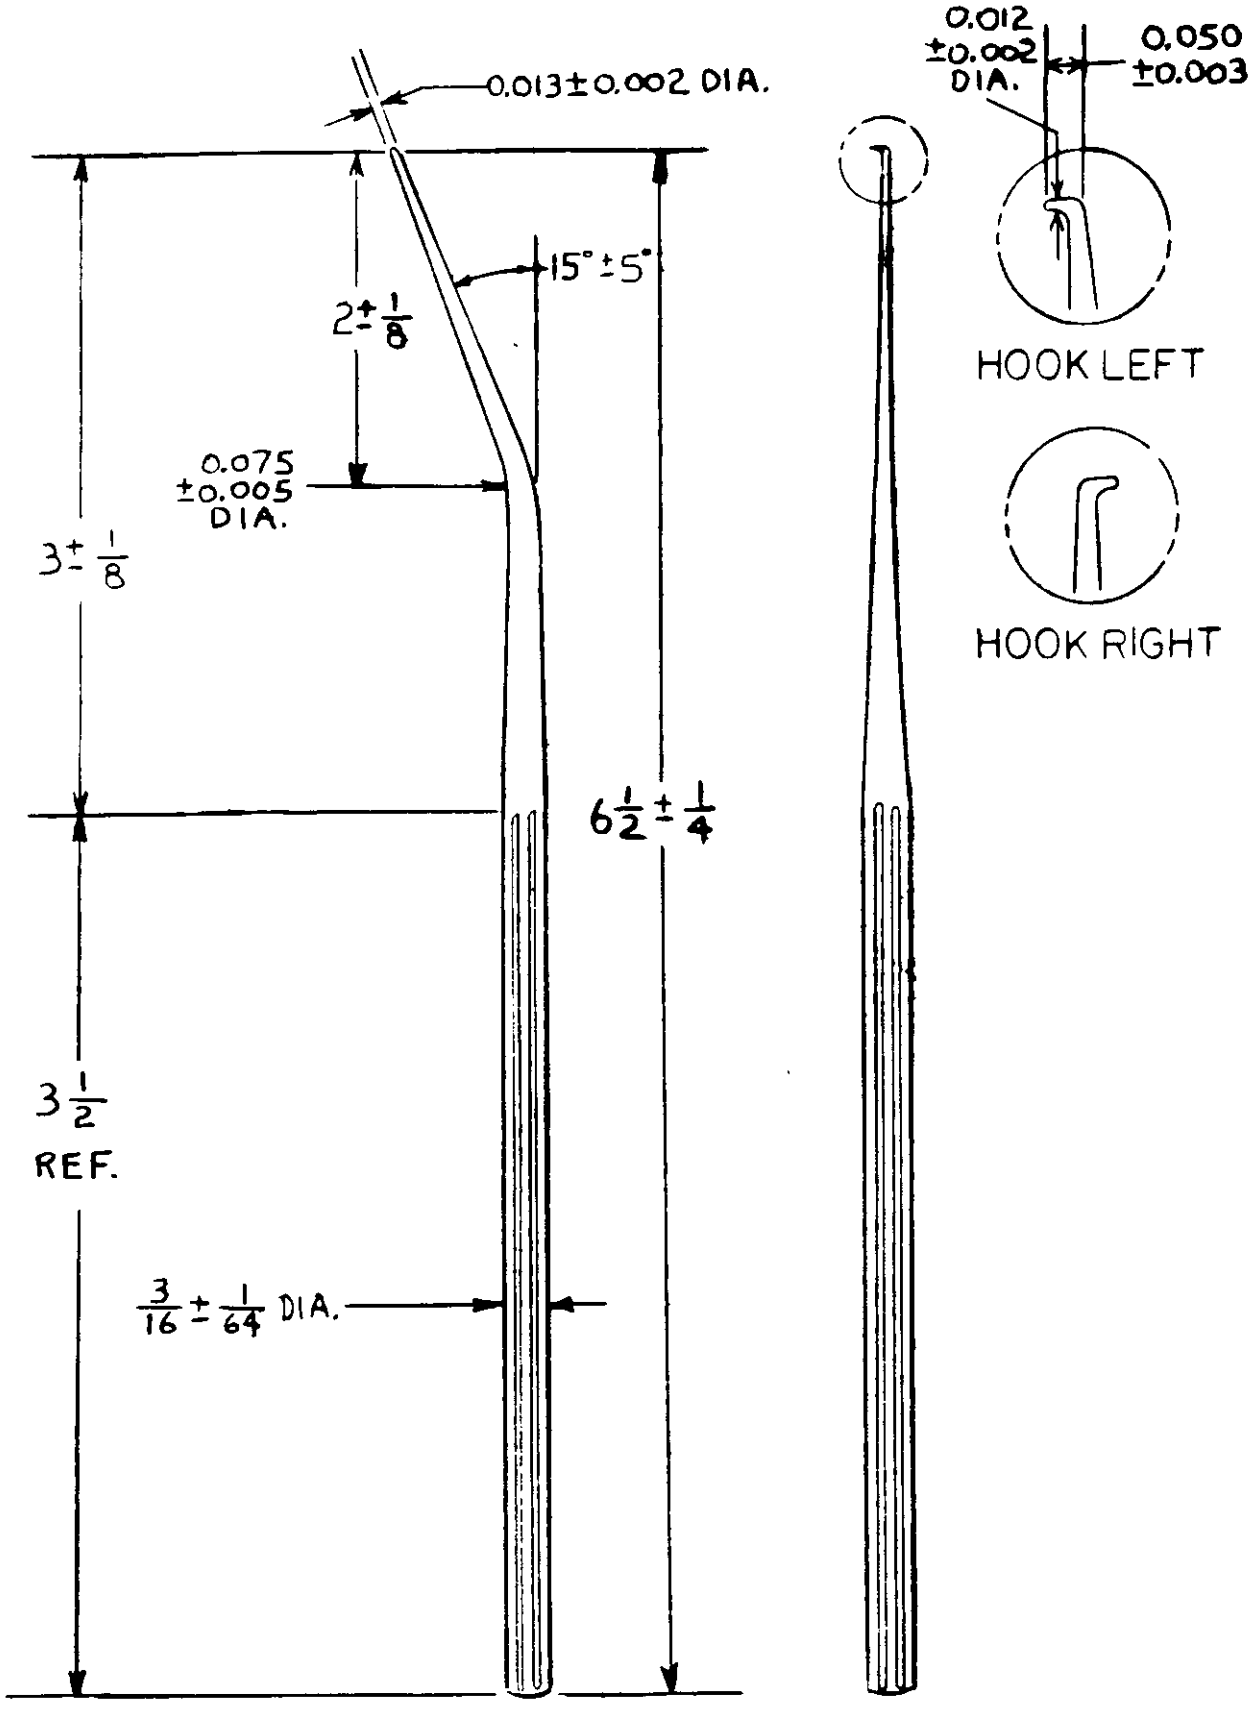


FIGURE 1 HOOK, INCUS, HOUSE 6515-01-139-8343-L 8344-R

☆U.S. GOVERNMENT PRINTING OFFICE: 1988 — 605-036/44950

Source: https://assist.dla.mil -- Downloaded: 2024-10-26T08:39Z
Check the source to verify that this is the current version before use.