NNN-F-001601 (DSA-DM)
August 19, 1969

INTERIM FEDERAL SPECIFICATION

FORCEPS, PINNING, ENTOMOLOGICAL SPECIMEN

This Interim Federal Specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. General Services Administration has authorized the use of this Interim Federal Specification.

1. SCOPE.

1.1 Scope. This specification covers curved forceps with blunt points suitable for use in pinning entomological specimens.

2. APPLICABLE DOCUMENTS

2.1 Specifications and Standards. The following documents, of the issue in effect on date of invitations for bid or requests for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

QQ-C-320	Chromium Plating (Electrodeposited).
QQ-N-290	Nickel Plating (Electrodeposited).
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.

FSC 6640

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

STANDARDS

Federal

FED-STD-66	Steel; Chemical Composition and Hardenability.
FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D. C. 20402

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Fort Worth, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

SPECIFICATIONS

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.
MIL-P-116	Preservation, Methods of.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

(Copies of Military specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

Standard Methods of Test for ROCKWELL HARDNESS AND ROCKWELL SUPERFICIAL HARDNESS OF METALLIC MATERIALS

ASTM Designation: E 18.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa. 19103)

3. REQUIREMENTS

3.1 Material. Material shall be carbon steel complying with FED-STD-66, AISI No. 1010 or No. 1020. Steel shall be nickel or chrome over nickel plated steel in accordance with QQ-N-290 and QQ-C-320.

3.2 Style and Design. Style and design shall be in accordance with Figure 1. Legs shall be double spot welded. Handles shall have forged, corrugated serrations to permit a firm finger grip. Tip serrations shall be double file-cut or stamped to insure firm grasp of entomological specimens and pins.


3.3 Hardness. The areas of greatest reduction in thickness (the tips, the springs) shall have Rockwell hardness from B-88 to B-105, and the thicker areas (handles) shall have Rockwell hardness from B-75 to B-80, when tested as specified in 4.4.1.

3.4 Corrosion resistance to boil. There shall be no signs of corrosion on the smooth surface of the forceps, when tested as specified in 4.4.2. A slight corrosion in the tip serrations shall not be cause for rejection.

3.5 Dimensions. Dimensions shall be in accordance with Figure 1.

3.6 Workmanship. Workmanship shall be first class throughout. The forceps shall be free from defects listed in Table III and other defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

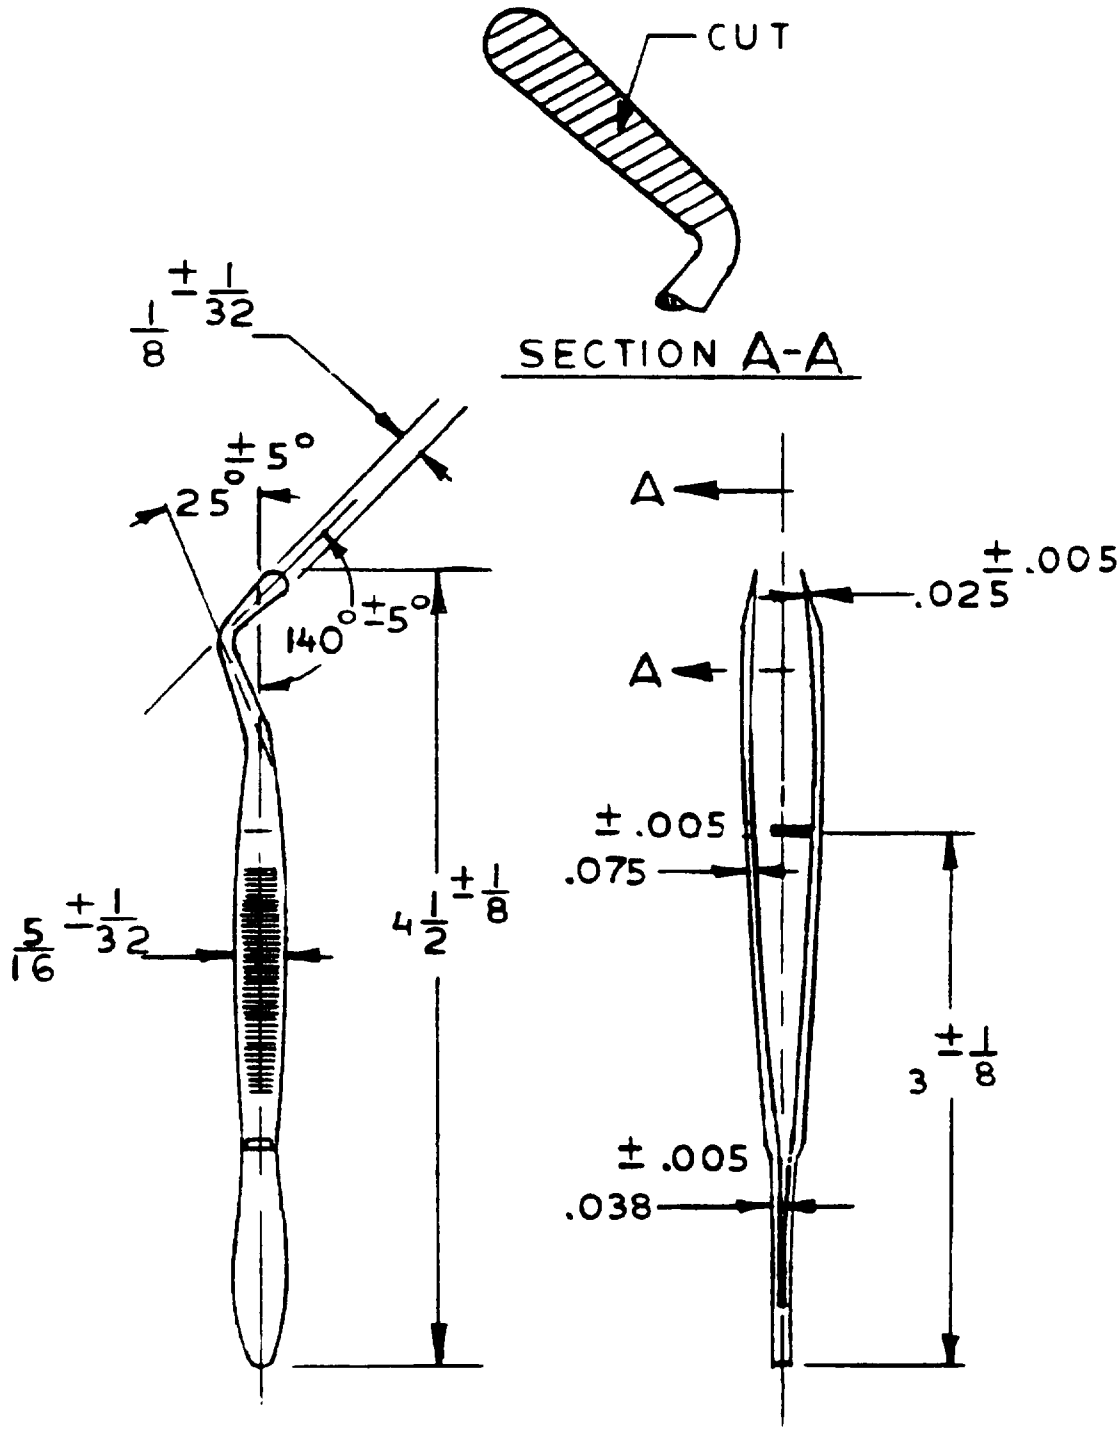

NOTE: ALL DIMENSIONS ARE IN INCHES

FIGURE 1 - FORCEPS, PINNING, ENTOMOLOGICAL SPECIMEN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of Quality. Certificates of quality, supplied by the manufacturer of the carbon steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL) shall be as indicated in Table I. Unit of product shall be one forceps.

Table I. Samrling for Examination

Type defect	Inspection level	AQL (percent defective)
For visual examination		
Major	II	1.0
Minor	II	2.5
For dimensional examination	S-2	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table II, except that the acceptance number shall be zero for all tests. Unit of product shall be one forceps.

Table II. Sampling for Tests

Characteristic	Requirement	Test procedure	Inspection level
Hardness	3.3	4.4.1	S-2
Resistance to boiling	3.4	4.4.2	S-2

4.3 Examination. The forceps shall be examined to determine compliance with all requirements contained in this specification. The forceps shall be examined for defects including, but not limited to, those listed in Table III.

Table III. Classification of defects

Categories	Defects
Major	
101	Guide pin not aligned with hole.
102	Plating not complete.
103	Forceps not free of cracks.
Minor	
201	Plating not free of blisters, or porosity.

4.3.1 Dimensional examination. The forceps shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Hardness test. Hardness shall be determined in accordance with ASTM Designation E 18.

4.4.2 Boil test. Before testing, the forceps shall be scrubbed with soap and water, rinsed thoroughly in distilled water, and dried. After cleaning, the forceps shall be boiled in distilled water, in a glass beaker, for 30 minutes and allowed to remain submerged for an additional 24 hours.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.1).

5.1.1 Unit of issue. One forceps, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be over-packed in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive materials.

5.1.3.4 Unit package. Each unit shall be packed in accordance with MIL-P-116, method IA-8.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers, of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.1).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table III, using type I, class I plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.2. Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, Table II, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with appendix of applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers, of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

a. Title, number, and date of this specification.

b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.