INTERIM FEDERAL SPECIFICATION

HOLDER, BLOOD COLLECTING TUBE

This Interim Federal Specification was developed by the General Services Administration, Federal Supply Service, Washington, D. C. 20406, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

1. SCOPE

1.1 This specification covers one type of plastic, blood-collecting tube holder, suitable for use with evacuated blood-collecting tubes, and double-pointed blood-collecting needles.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

Federal Specifications:

L-P-394 - Plastic Molding Material (Propylene Plastics, Injection and Extrusion).
PPP-B-636 - Box, Fiberboard.

Federal Standards:

Fed. Std. No. 123 - Marking for Domestic Shipment (Civil Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other Federal specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Offices in Boston, New York, Washington, D.C., Atlanta, Chicago, Kansas City, Mo., Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, Washington.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies).

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

FSC 6630

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless a specific issue is identified, the issue in effect on date of invitation for bids or request for proposal shall apply.

National Classification Board:

National Motor Freight Classification.

(Application for copies should be addressed to the American Trucking Association, Inc., Attn: Tariff Order Section, 1616 P Street, N. W., Washington, D. C. 20036.)

Uniform Classification Committee:

Uniform Freight Classification.

(Application for copies should be addressed to the Uniform Classification Committee, 202 Union Station, Chicago, Illinois 60606.)

3. REQUIREMENTS

3.1 The holders shall be fabricated of translucent polypropylene plastic in accordance with L-P-394.


3.2 Construction and design. The holders shall be constructed in accordance with Figure 1. One end of the holder shall be entirely open for the free insertion of a vacuum blood-collecting tube. The open end shall have a flange around its periphery suitable for an ample finger hold. Opposite segments of the flange shall be shaped so as to check rolling. The opposite end of the tube shall be closed except for a centrally located passage, threaded so as to form a secure fit with the double-pointed, blood-collecting needles. A permanent guideline, perpendicular to the vertical axis of the holder, shall be located 7/32 inch from the inside bottom of the threaded end. The guideline shall be situated so that after the needle is screwed into the holder and the tube is inserted so that the top of the stopper meets the guideline, the rear point of the needle shall be imbedded in the diaphragm and shall not puncture it.

3.3 Dimensions. The dimensions of the holders shall be in accordance with Figure 1.

3.4 Identification marking. Each holder shall be legibly and permanently marked with the name or registered trademark of the manufacturer.


3.5 Workmanship. Workmanship shall be first-class throughout. The holder shall be free from defects which detract from its appearance or may impair its serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

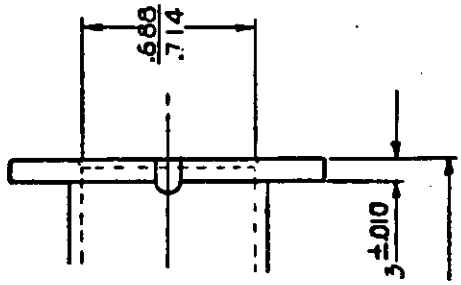

3E

.1865-16 SPECIAL DOUBLE THD. ⅛ LEAD.

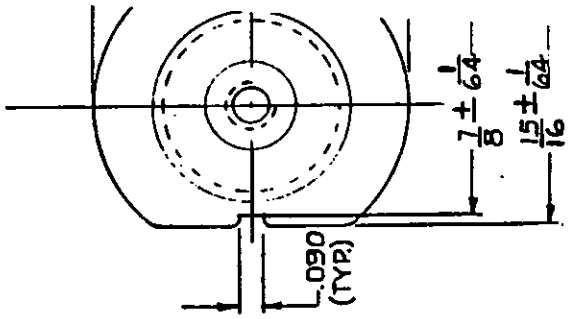

FIGU

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to insure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as shown below.

Sampling for examination

Examination	Inspection level	AQL (percent defective)
For visual examination:		
Major defects	II	2.5
Minor defects	II	4.0
For dimensional examination	S-1	2.5

4.3 Examinations. The holders shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects.

Classification of defects

Category	Defect*
Major	
101	Holder not free from burrs or sharp edges.
102	Holder not free from cracks, chips, or blisters.
103	Holder not free from deformation.
104	Thread not free from breaks.
105	Guideline not visible or permanent.
106	Holder not free from dirt, grease, or foreign particles.
Minor	
201	Identification marking not present, complete, correct, legible, or permanent.

*Examination shall not be restricted to the classified possible defects listed above.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

4.3.2 Dimensional examination. The holders shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing and marking comply with the requirements of section 5. Defects shall be scored as specified in table I. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of defects per hundred units.

TABLE I. Examination of preparation for delivery

Examine	Defect
Containers	Not as specified.
Contents	Not as specified.
Markings	Omitted, incorrect; illegible; improper size, location, sequence or method of application.
Materials	Component missing or damaged.
Workmanship	Bulging or distortion of containers. Cushioning inadequate, improper or missing.

4.4.1 Examination for closure of shipping containers. When shipping containers are required to be in accordance with PPP-B-636, examination for defects in closure shall be in accordance with the appendix of that specification.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level B or C, as specified (see 6.2).

5.1.1 Level B. Twelve holders shall be packaged in a snug-fitting carton of the type normally used for the item.

5.1.2 Level C. Holders shall be packaged to afford adequate protection against damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level B or C, as specified (see 6.2).

5.2.1 Level B. Forty-eight cartons shall be packed in a snug-fitting box conforming to PPP-B-636 class domestic.

5.2.2 Level C. Holders in quantities as specified (see 6.2), packaged as specified in 5.1 shall be packed in containers to assure carrier acceptance and safe arrival at destination in compliance with the Uniform Freight Classification or National Motor Freight Classification, as applicable.

5.3 Marking. In addition to any special markings required in the procurement document, marking of the interior packages and exterior shipping containers shall be in accordance with Fed. Std. No. 123 for civil agencies or MIL-STD-129 for military agencies, as applicable (see 6.2).

6. NOTES

6.1 Intended use. The holder is intended for use with the following items: Blood collecting, hypodermic needles; and blood collecting tubes, vacuum, sterile and nonsterile, with and without anticoagulant.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Purchaser should select the preferred options permitted herein and include the following information in procurement documents:

(a) Level of packaging and packing required (see 5.1 and 5.2).

(b) Marking document required (see 5.3).

GSA DC 71.3535

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.

GENERAL SERVICES ADMINISTRATION - FEDERAL SUPPLY SERVICE

SPECIFICATION COMMENT SHEET

BUDGET BUREAU NO. 29-R0175

INSTRUCTIONS

This form provides a way for users of this specification to inform the originator of problems encountered in its use. It is not to be used to request changes to accommodate proprietary features. All comments will be considered and appreciated, but please do not expect a reply. To comment: detach, complete, and mail to: General Services Administration, FSS (FMSC), Wash., D.C. 20406.

NOTE: Comments on this form do not constitute or imply authorization to waive any part of the document or serve to amend contractual requirements.

1. SPECIFICATION

NNN-H-001497(GSA-FSS) Holder, Blood Collecting Tube

2. CONTRACT NO. *(If any)*	3. QUANTITY ON CONTRACT *(Optional)*	4. DOLLAR VALUE *(Optional)*

5. GENERAL NATURE OF PROBLEM *(e.g., inspection difficulties, manufacturers unable to meet tolerances, containers collapse under normal warehousing conditions, etc.)*

6. SPECIFIC REQUIREMENTS AFFECTED *(Include paragraph number and lines of wording)*

7. SPECIFIC PROBLEMS *(e.g. tests in 4.2.2 will not assure that the battery will last required time; temperature ranges in table 2 do not conform to commercially available items.)*

8. RECOMMENDATIONS

9. NAME OF MANUFACTURER, ASSOCIATION, GOVT., AGENCY, ETC.	10. ADDRESS *(Number, Street, City, State and Zip Code)*

11. NAME AND TITLE OF SUBMITTER	12. DATE

FORM GSA FEB 69 2200

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:49Z
Check the source to verify that this is the current version before use.