A-A-51365A
23 September 1987
SUPERSEDING
A-A-51365
24 March 1987

COMMERCIAL ITEM DESCRIPTION

CANNULA, EAR (House, Suction-Irrigator)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers House ear suction-irrigator cannulas used for middle ear surgical procedures.

Salient characteristics:

General. The cannula shall have a suction tube with a finger tip control, an irrigator tube, and two obturators (one for each tube), for use in middle ear surgical procedures.

Material. The cannula shall be fabricated from Class 3 austenitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The cannula shall have a Rockwell hardness of B85 minimum.

Style and design. The cannula shall be of the House suction-irrigator design. The suction lumen shall have a finger tip control on the shaft 2.8 ± 0.3 cm from the proximal end. The by-pass hole on the finger device shall have the same nominal cross-sectional area as the inside of the suction lumen shaft. At the proximal end of each cannula, there shall be an enlarged section suitable for connection of tubing. The finger device and both tubing connectors shall be permanently attached to the cannula shaft. The irrigation lumen shall be permanently attached to the suction cannula. The style and dimensions shall be in accordance with Figure 1. The cannula shall be free from any sharp edges or cracks.

Obturator. When inserted into the lumen, the obturator shall be long enough to pass completely through the cannula and tubing connector. The proximal end of the obturator shall provide a non-slip grip, or shall be formed into a loop.

Passivation. The cannula shall be properly passivated.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Finish. The finish shall be satin or mirror in accordance with Federal Specification GG-I-526. The finish shall be uniform and free from burs, scale, corrosion, pits, and rough areas.

Identification Markings. The cannula shall bear the name or registered trademark of the manufacturer, the word "stainless", and the French size. Cannulas of foreign manufacture shall also bear the name of the country of manufacture.

Workmanship. The cannula shall be free from defects which detract from its appearance or impair its serviceability.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements. The surface of the cannula shall be smooth and lumina void of obstruction.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (Ea). One cannula, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for visual examination shall be in accordance with MIL-STD-105. The unit of product for examination shall be one cannula. Sampling shall be Level II with an AQL of 6.5

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for Tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one cannula. AQL shall be 1.0 percent defective. Inspection level shall be S-2.

Corrosion resistance test. Cannulas shall be tested for corrosion resistance in accordance with the Resistance to Boil test of Federal Specification GG-I-526.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-769-1075	CANNULA, EAR, HOUSE, Medium 16 X 18 Gage
6515-01-111-5050	CANNULA, EAR, HOUSE, Suction-Irrigator, 4 X 5 Fr, Large
6515-01-112-6415	CANNULA, EAR, HOUSE, Suction-Irrigator, 8 X 12 Fr, Medium
6515-01-112-6416	CANNULA, EAR, HOUSE, Suction-Irrigator, 6 X 8 Fr, Medium
6515-01-112-6417	CANNULA, EAR, HOUSE, Suction-Irrigator, 12 X 14 Fr, Medium
6515-01-112-6418	CANNULA, EAR, HOUSE, Suction-Irrigator, 7 X 10 Fr, Medium
6515-01-112-6419	CANNULA, EAR, HOUSE, Suction-Irrigator, 5 X 7 Fr, Large
6515-01-114-5498	CANNULA, EAR, HOUSE, Suction-Irrigator, 5 X 7 Fr, Medium
6515-01-139-8305	CANNULA, EAR, HOUSE, Suction-Irrigator, 6 X 8 Fr, Large

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4057

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

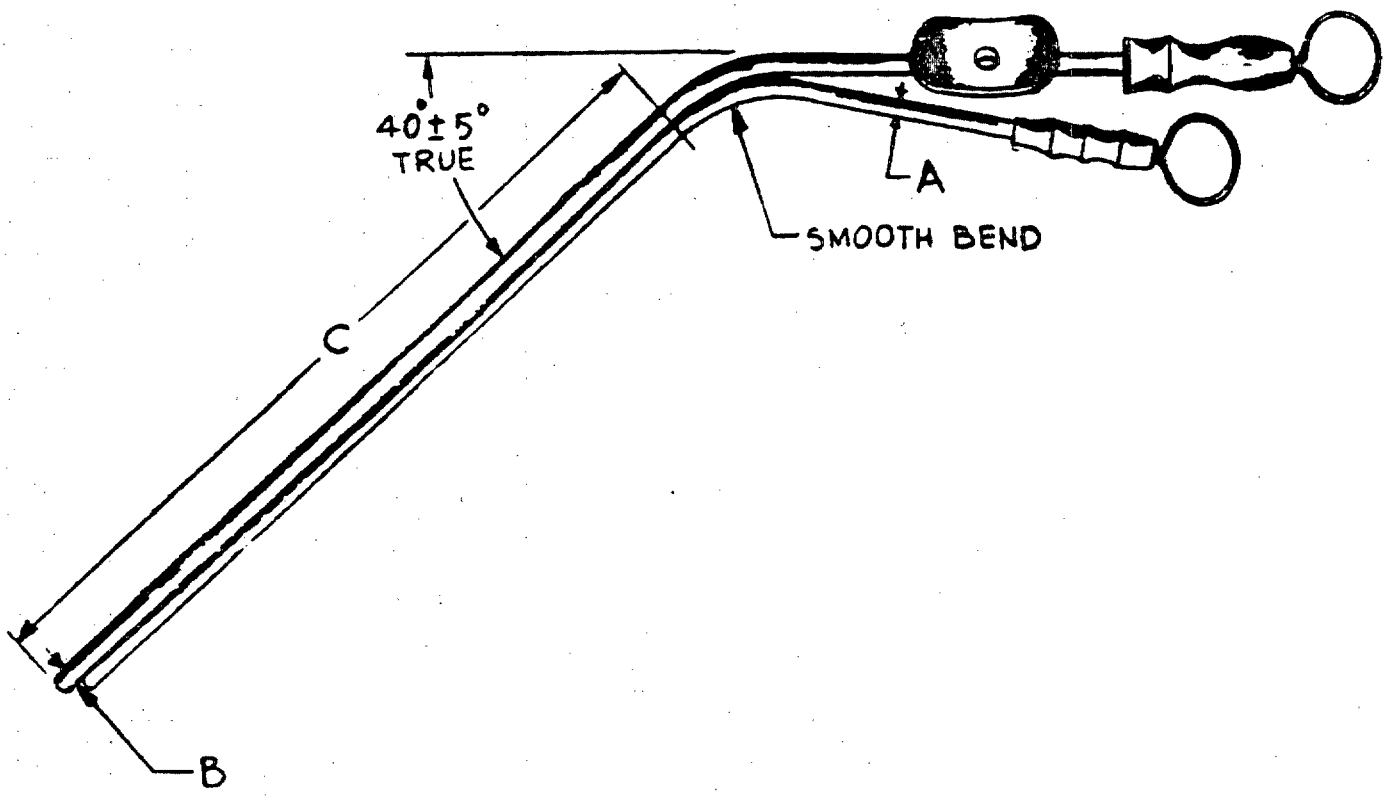

NSN	A (FR. SIZE)	B (FR. SIZE)	C (LENGTH)
6515-01-111-5050	4	5	9.5±.7CM
6515-01-112-6415	8	12	7.2±.5CM
6515-01-112-6416	6	8	7.2±.5CM
6515-01-112-6417	12	14	7.2±.5CM
6515-01-112-6418	7	10	7.2±.5CM
6515-01-112-6419	5	7	9.5±.7CM
6515-01-114-5498	5	7	7.5±.5CM
6515-01-139-8305	6	8	9.5±.7CM
6515-00-769-1075	4	5	7.2±.5CM

FIGURE 1 CANNULA, EAR, HOUSE, SUCTION-IRRIGATOR

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51365A	CANNULA, EAR (House, Suction-Irrigator)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
3b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426

PREVIOUS EDITION IS OBSOLETE.

(FOLD ... H THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.