A-A-51448A
30 May 1989
SUPERSEDING
A-A-51448
30 May 1986

COMMERCIAL ITEM DESCRIPTION

TABLE, SURGICAL INSTRUMENT AND SURGICAL DRESSING

Angular-Top

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Type I of Federal Specification AA-T-55B which is cancelled.

This Commercial Item Description covers a corrosion-resisting steel angular-top surgical instrument and surgical dressing table.

Salient characteristics:

The surgical instrument and surgical dressing table, having an angular table top, shall be fabricated of American Iron and Steel Institute (AISI) Series 300 corrosion-resisting steel. The table shall have a width of 15 inches plus or minus 1 inch, with a height of 34-1/2 inches plus or minus 1/2 inch. The table top shall be angled at 135° plus or minus 2° with a 72 inch plus or minus 1 inch dimension between the two outer rear uprights as shown in figure 1.

The table shall be supported by six uprights, or legs, of 1 inch diameter by 0.049 inch minimum wall thickness corrosion-resisting steel tubing located one at each corner and one each at front and back center of the table. The uprights shall be reinforced by bracing of 1/2 inch solid corrosion-resisting steel rod or 3/4 inch outside diameter by 0.049 inch wall thickness corrosion-resisting steel tubing welded to all six legs with cross bracing approximately 7 inches above the floor, as shown in figure 1.

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

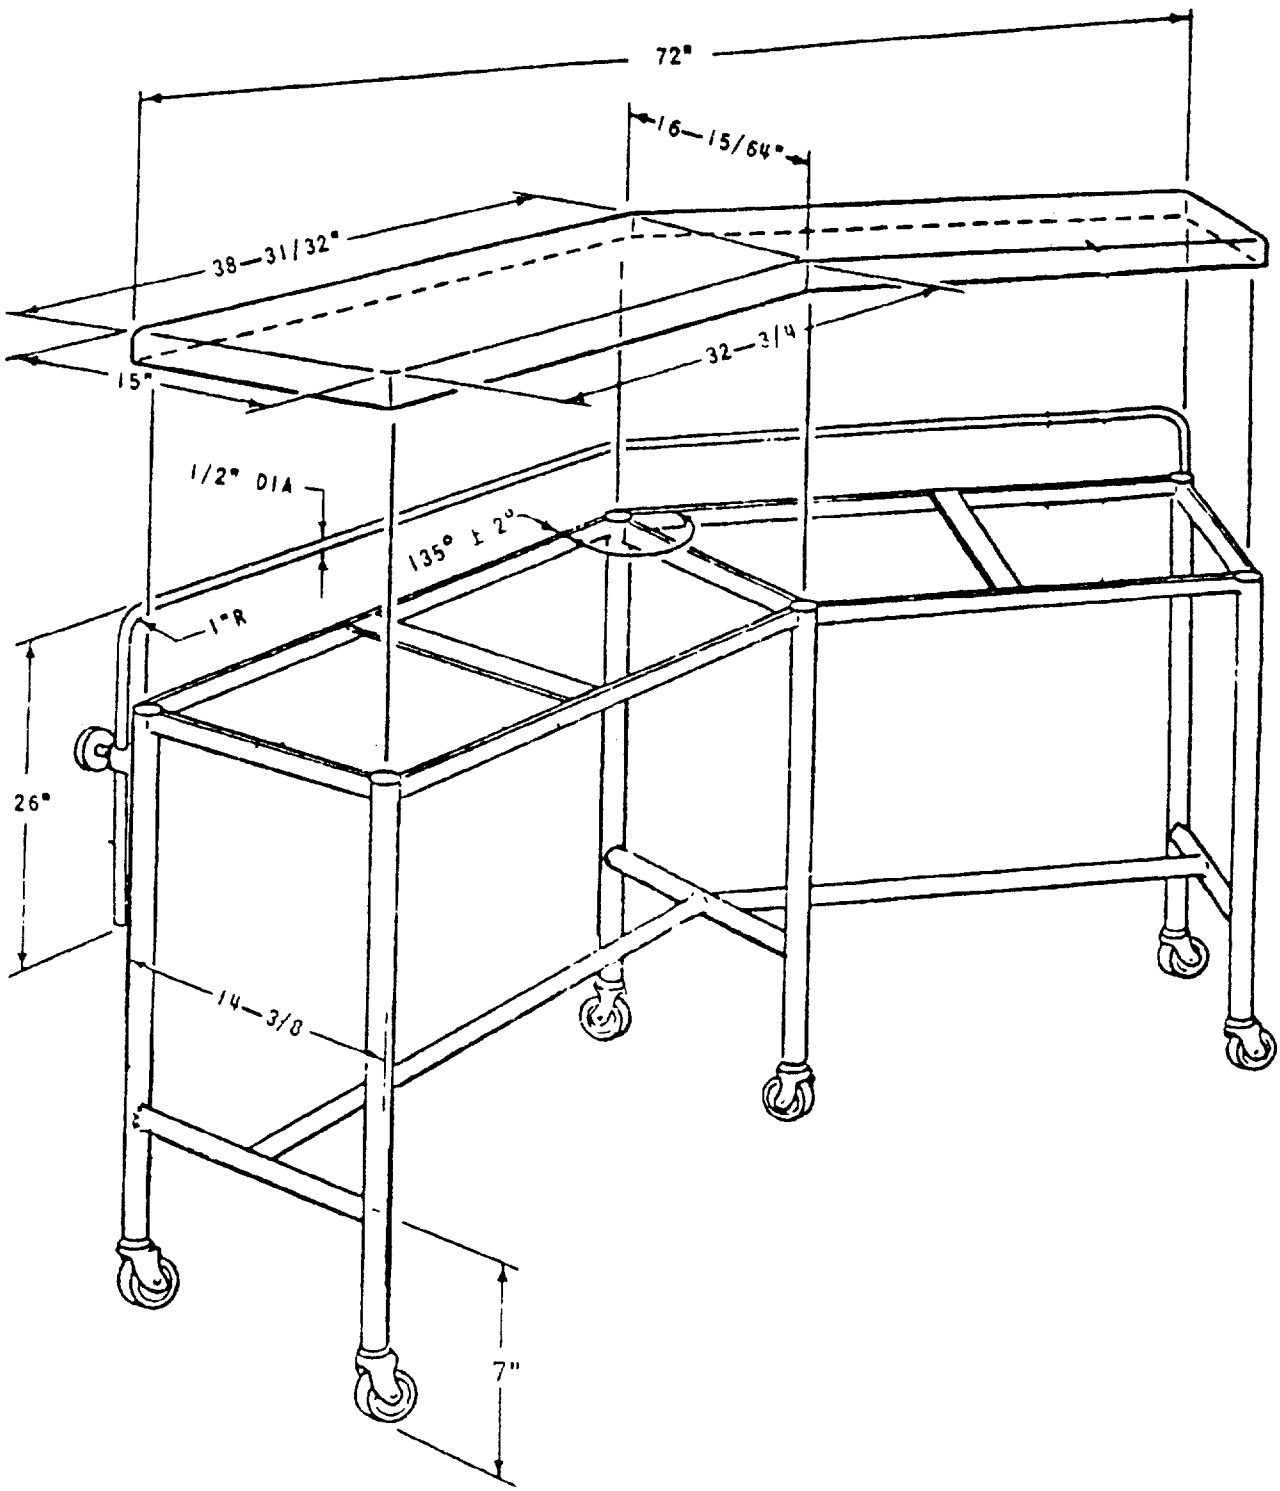


FIGURE 1. Angular-top table.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

The six table legs shall each be fitted with a swivel-type, 3 inch minimum diameter, 3/4 inch minimum width, electrically conductive caster. Two outer casters on the long axis of the table shall have a brake. Each caster shall have a nominal load rating of 75 pounds.

The table top shall be made of corrosion-resisting steel 0.0625 inch thick (No. 16 United States Standard Gage). All edges of the top shall be flanged downward approximately 1-1/8 inch and hemmed approximately 3/8 inch. The top shall be continuously welded at all vertical contact points with the uprights the full distance of the turndown. As an alternate, the table top may be fabricated of corrosion-resisting steel a minimum of 0.035 inch thick (No. 20 United States Standard Gage), if supported by a reinforcing framework of 1 inch wide by 0.079 inch thick (no. 14 U.S.S. Gage) corrosion-resisting steel as shown in figure 1. In lieu of the reinforcing framework a carbon steel subtop, a minimum of 0.0475 inch thick (No. 18 U.S.S. Gage), having the underside coated with an acrylic enamel finish, may be attached to the corrosion-resisting steel top by means of studs.

The table shall have an adjustable curtain rail constructed from a 1/2 inch diameter solid corrosion-resisting steel rod. The rail shall be adjustable to a height of 12 inches above the table top.

The table shall be of welded construction throughout. The welding rods shall be corrosion-resisting steel similar in composition to the welded members. The surfaces to be welded shall be free from grease, oil, oxides or other foreign matter. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag or excessive spatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement. All welds shall be continuous with no visible voids, pin holes, or cracks.

All exposed corners and edges shall be broken, rounded, or otherwise treated to eliminate sharp edges. All exposed corrosion-resisting steel surfaces shall be free from pit marks, weld seams, scale, and shall have a No. 4 commercial finish. The finish shall be uniform and free of coarse grind marks and scratched areas.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

The table shall be furnished clean and free of oil, grease, dirt, or other contamination. The assembled table shall meet the electrical conductivity requirements of the National Fire Protection Association (NFPA) Code No. 99, Health Care Facilities.

Workmanship. The surgical instrument and surgical dressing table shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One table, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one surgical instrument and surgical dressing table, as specified in this description.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Defects.

Table is not complete with all components.

Table does not sit evenly on a flat surface.

Casters do not swivel or roll smoothly, quietly, or evenly.

Exposed welds are not ground smooth to blend with adjacent surfaces.

Welds are not continuous, not clean, or not free of pitting, splatter, or discoloration.

Exposed or accessible edges, corners, or surfaces, are not free of burrs, sharpness, or sharp projections.

Finish is not uniform and free of coarse grind marks or scratched areas.

Table is not clean and free of oil, grease, dirt, or other contamination.

Sampling for tests. Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-3. The unit of product for test purposes shall be one surgical instrument and surgical dressing table.

a. First article. Where a first article sample is required, all tests shall be performed on that unit.

b. Acceptance testing. When a first article sample has not been required, one unit shall be subjected to the performance test specified herein. If a test article sample has successfully passed all tests, performance test shall not be required at acceptance.

Tests.

Electrical conductivity. The assembled table, complete with casters, shall be tested in accordance with National Fire Protection Association (NFPA) Standard No. 99, Health Care Facilities. Failure to meet electrical conductivity standards shall constitute a defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6530-00-709-3960

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6530-2072

Location:
CID/TABLE/SURGICAL/INSTRU/H13-19

☆U.S. GOVERNMENT PRINTING OFFICE: 1989 - 604-833/[illegible]

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS. In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4956 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC- RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

NO POSTAGE
NECESSARY
IF MAILED
IN THE
UNITED STATES

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51448A	TABLE, SURGICAL INSTRUMENT AND SURGICAL DRESSING, Angular-Top

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426

PREVIOUS EDITION IS OBSOLETE.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.