A-A-51690A
19 February 1988
SUPERSEDING
A-A-0051690(DM)
26 September 1986

COMMERCIAL ITEM DESCRIPTION

MASK, ORONASAL (Plastic, Elongated)

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a disposable, elongated oronasal oxygen mask.

Salient characteristics.

The mask shall be manufactured from a green-tinted transparent vinyl plastic. The mask shall be an elongated adult size with dimensions in accordance with Figure 1. The mask shall be contoured to fit the human face. The mask shall have an adjustable elastic headband 18 inches in length (minimum). The mask shall be of the non-rebreathing design. The mask connector shall have a rubber washer on the mask end which allows entry of air into the mask but which seats on the connector and prohibits flow of exhaled gasses into the connector. The connector shall make a leak-proof connection with the mask, but shall not be cemented. The connector shall be capable of being turned in the mask socket such that the tubing nipple is capable of turning through an arc of 180 degrees.

The connector shall have a plastic reservoir bag attached to it on the end opposite the mask. The bag shall be capable of holding a minimum of 400 ml of oxygen. The connector shall have a integral divertor plate near the tubing nipple inlet which directs incoming oxygen into the direction of the bag.

The tubing nipple shall have 84 ± 10 inches of 3/16 ± 1/64 inside diameter tubing attached to it. The tubing shall be manufactured from green-tinted transparent polyvinylchloride plastic. The proximal end of the tubing shall have an attached connector capable of making a leakproof connection to a standard oxygen regulator nipple.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

The plastic material shall not irritate the skin when tested in accordance with the safety (skin irritation) test.

Workmanship. The mask shall be processed in such a manner as to be uniform and free from defects that will affect life, serviceability, or appearance.

Product Quality Level

Visual and dimensional examination. Masks shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Package (PG). One package containing 50 masks, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Safety (skin contact) test. Apply a 0.5 inch by 0.5 inch piece of the face mask to the skin on the body side of the upper arm of five volunteers. The patch of plastic shall be held in place by means of a strip adhesive tape of a width not exceeding the width of the plastic sample. The plastic sample shall be allowed to remain in contact with the skin for 24 hours. The patch shall be removed from the contact area and no reaction shall be visible. Within an additional 24 hours there shall be no delayed reaction on any of the subjects. If the patch unduly irritates the skin, the patch shall be removed immediately.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Alternate safety (skin contact) test. The manufacturer may submit an alternate test protocol for the Safety Test to the Directorate of Medical Materiel, ATTN: DPSC-RST, DPSC, 2800 S. 20th Street, Philadelphia, PA 19101. If the alternate test is deemed acceptable, the manufacturer shall be issued a letter-of-equivalency, and the alternate test may be used in lieu of the Safety Test above on that and future contracts. The protocol shall include a description of the method, apparatus, positive and negative controls, and acceptance/rejection criteria.

Certificates of safety. A certificate of compliance, stipulating that offered items meet the safety test, shall be acceptable, provided that the contractor has supplied acceptable items to the Government within the past three years, and that there have been no changes to material formulation and method of processing since actual testing was performed. The certificate shall include the date of actual testing, the test method and results, the name and title of the person evaluating results, the current contract number and NSN, a statement to the effect that material processing and formulation have not changed since actual testing was performed, and the signature and title of the person making the certification.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-164-3755	MASK, ORONASAL.

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 50979

Project No. 6515-4002

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

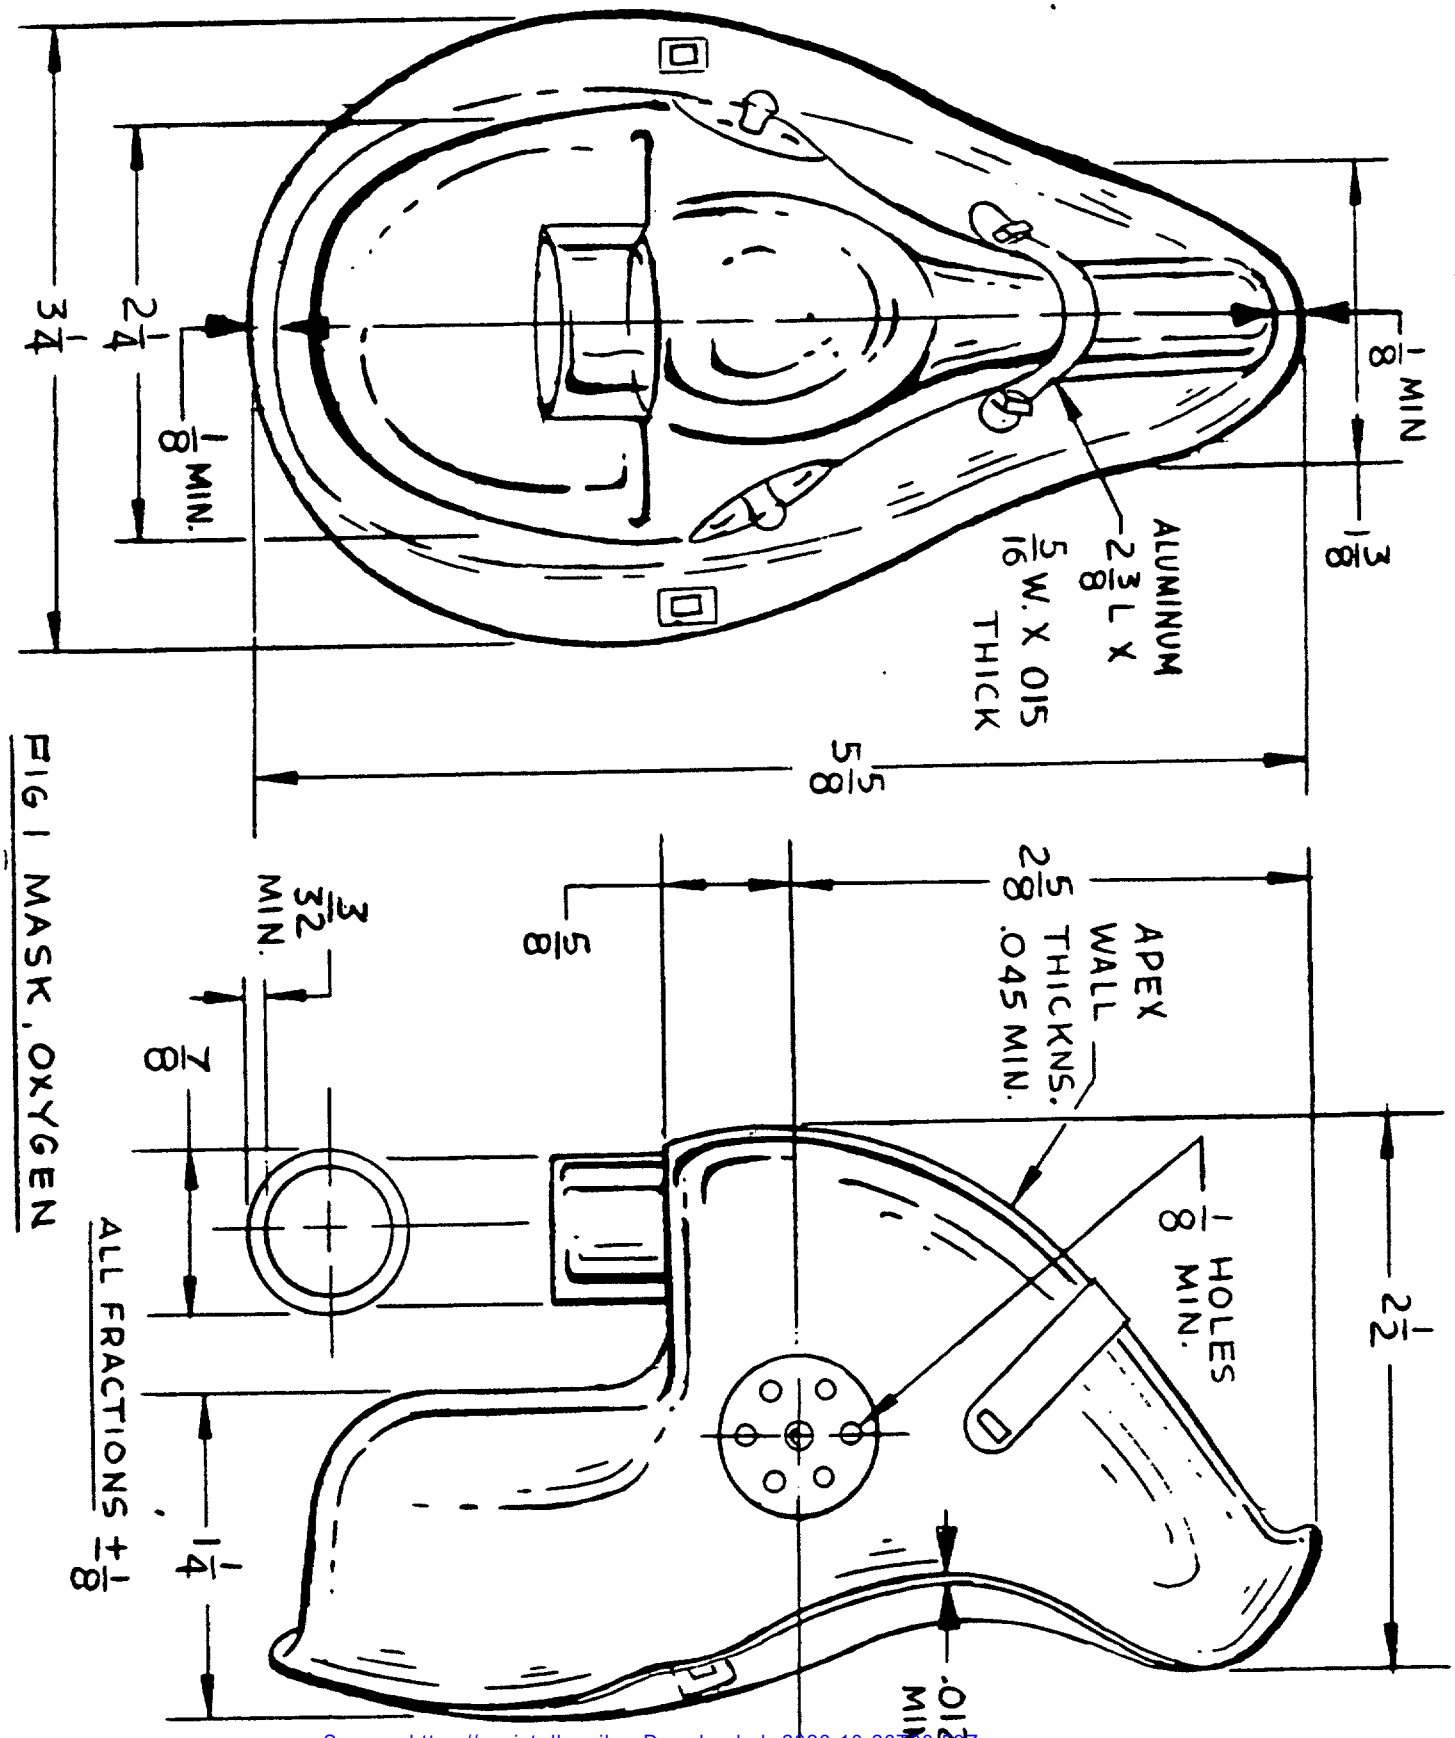


FIG 1 MASK, OXYGEN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.