A-A-51699
2 October 1986

COMMERCIAL ITEM DESCRIPTION

ADAPTER, SYRINGE

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers syringe adapters for use with twin wheel and flag handle endoscopes.

Salient characteristics:

General. The syringe adapter shall be designed to facilitate connection of a syringe to the working channel of twin wheel and flag handle endoscopes.The adapter shall fit those endoscopes that have working channels with inside diameters of 0.07 inch (1.8 mm) or larger.

Material. The adapter shall be fabricated from corrosion-resisting metal.

Characteristics. The proximal end shall have a female Luer lock adapter. The Luer lock adapter shall conform to the requirements of ANSI/HIMA MD70.1. The flange portion of the adapter shall be either knurled or coined. Near the distal end of the adapter there shall be two holes to allow flow. The cross sectional area of each hole shall be at least 75 percent of the cross sectional area of the inside diameter of the cannula. The adapter shall be in accordance with Figure 1.

Boil test. The adapter shall meet the boil test requirements as specified in Federal Specification GG-I-526.

Clear channel test. Fill a syringe with 5 milliliters (ml) of water. Attach the syringe to the adapter. Empty the syringe into the adapter and verify that the water flows through the syringe channel and out the distal end.

Workmanship. The syringe adapter shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (Ea). One syringe adapter, as specified, constitutes one unit.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for Tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one syringe adapter. Sampling shall be S-2, AQL 2.5.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-168-0556	ADAPTER, SYRINGE, Corrosion-Resisting Steel

This adapter is designed for use with American Cystoscope Maker endoscopes.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51699

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 58369

Project No. 6515-3429

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

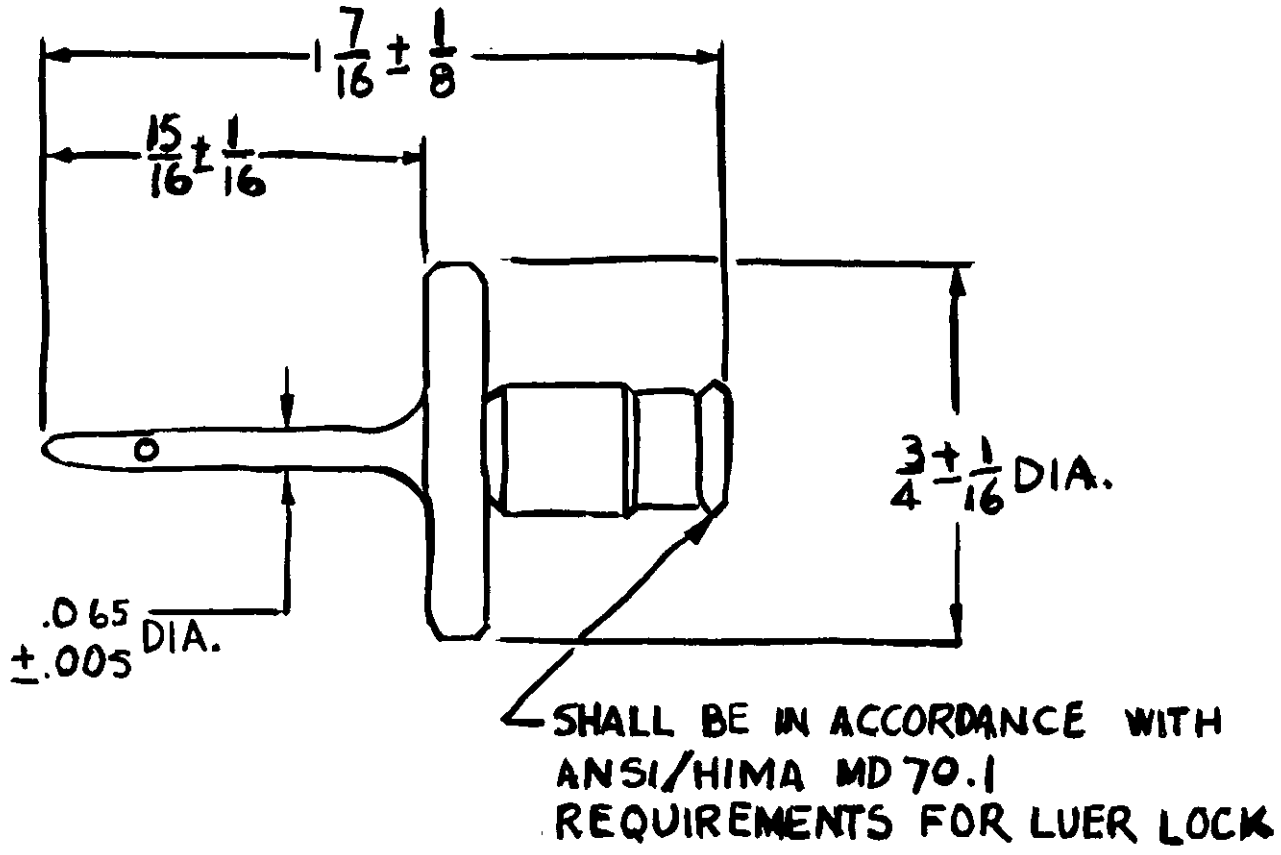

NSN 6515-01-168-0556

FIGURE 1 ADAPTER, SYRINGE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.