A-A-51701
24 November 1986

COMMERCIAL ITEM DESCRIPTION

MALLET, ORAL SURGERY (Gardner, Hand Type)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a dental mallet suitable for use in oral surgical procedures.

Salient characteristics:

Material. The mallet shall be fabricated of class 6, type 430F ferritic stainless steel, as specified in ASTM F899.

Hardness. The Rockwell hardness of the mallet shall be C25 to C30, tested as specified in ASTM E18 (Rockwell).

Style, design, and dimensions. The mallet shall be a Gardner type dental mallet suitable for use in oral surgical procedures. Shall be of two-piece construction with the head and handle permanently joined. The handle shall have two finger grip bands, longitudinally serrated, and raised above the surface of the shank. The weight of the mallet shall be 9.5 $\pm$ 0.5 ounces. The dimensions of the mallet shall conform to figure 1.

Finish. The mallet shall have a bright or matte finish.

Corrosion resistance. The mallet shall show no evidence of corrosion, after the boil test of GG-I-526.

Workmanship. The mallet shall be free from burrs and sharp edges or other defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One mallet, as specified, constitutes one unit.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

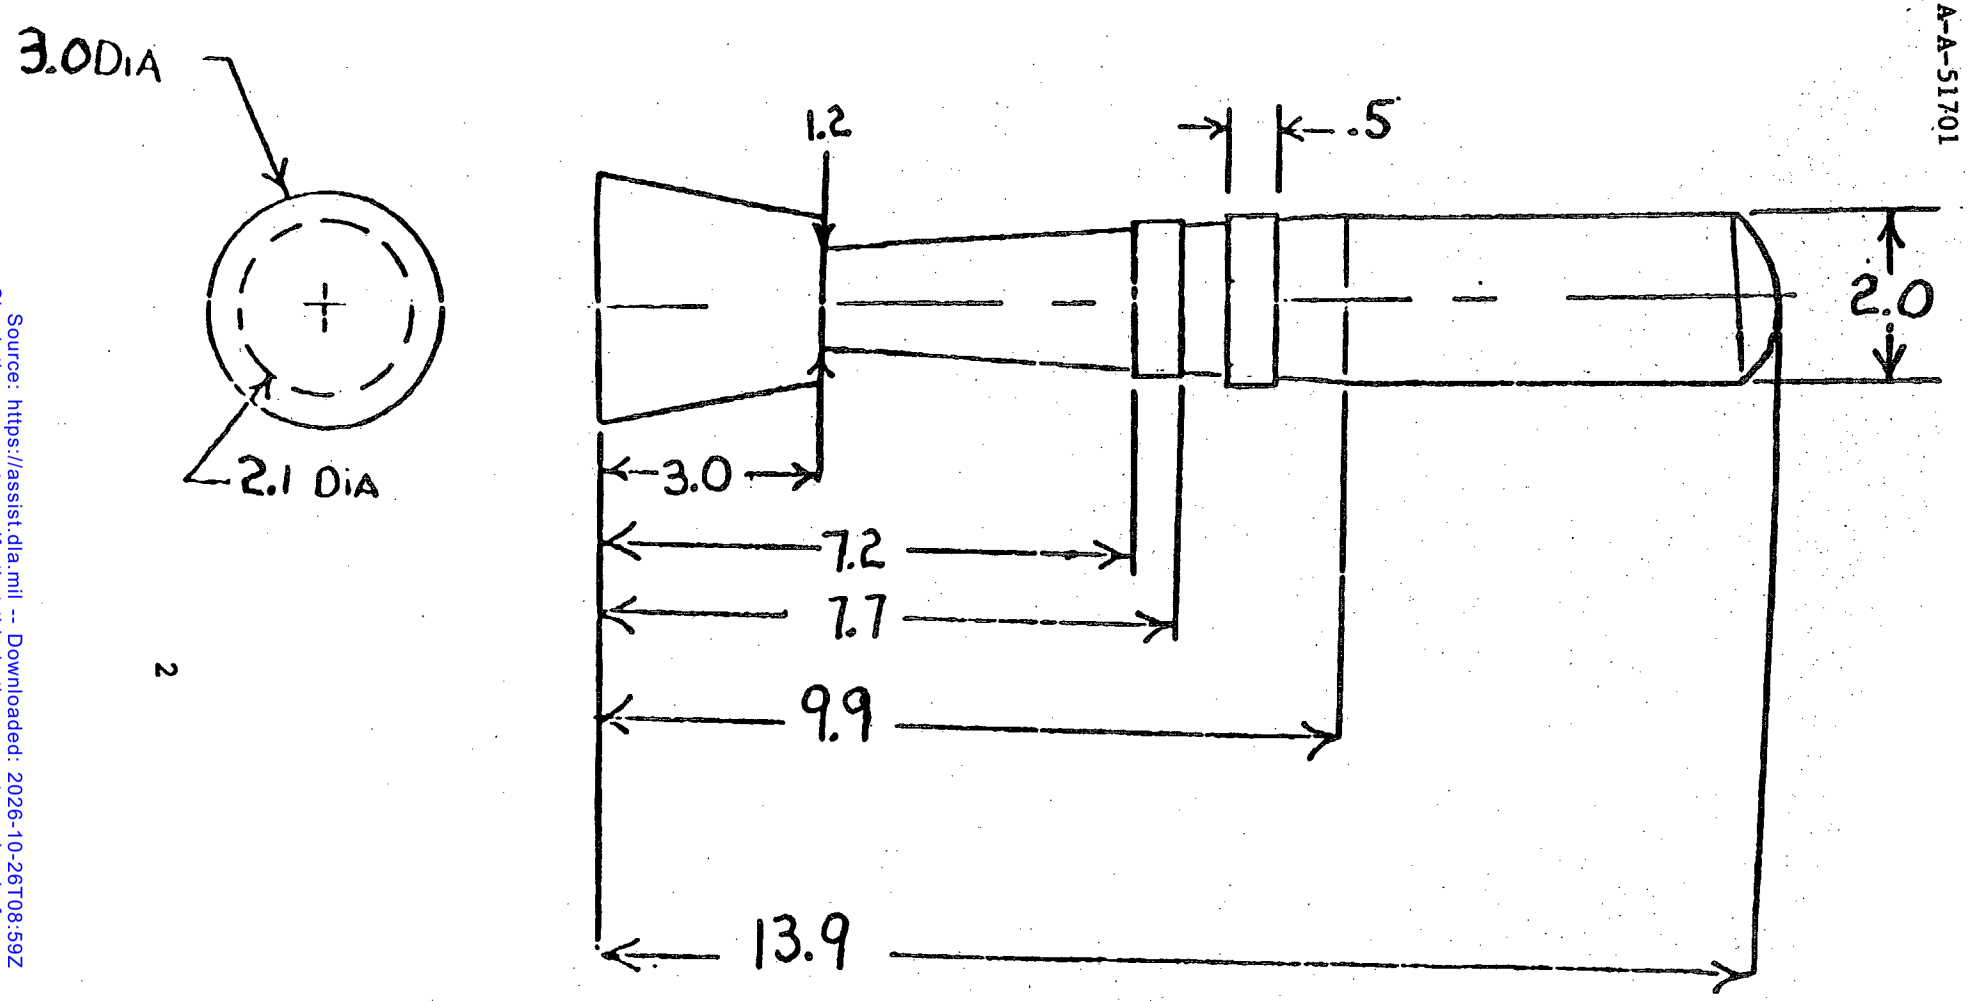


FIGURE 1. Mallet, Oral Surgery, Gardner

Note: All dimensions are in centimeters (cm) with tolerances of ± 5%.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one mallet. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

Stock Number	Item Identification
6520-01-058-5954	MALLET, ORAL SURGERY, Hand Type, Gardner, 9.5 Oz. (280.25 ml)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA - DM

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

PROJECT NO. 6520-1970

49043

Location: NCR Disk 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.