A-A-51702A
5 June 1987
SUPERSEDING
A-A-0051702(DM)
7 October 1986

COMMERCIAL ITEM DESCRIPTION

SPECULUM, SEPTUM (Cottle)

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers Cottle septum speculum for use in exposing the nasal canals.

Salient characteristics.

General. Shall be a septum speculum of the Cottle design for use in exposing the nasal canals.

Material. Except for the screws and pins, the speculum shall be fabricated from Class 4 martensitic corrosion-resisting steel. The screws and pins shall be fabricated from either austenitic corrosion-resisting Type 303 steel or martensitic corrosion-resisting steel. The chemical composition of the steel shall be in accordance with ASTM F899 for the class and type used.

Hardness. The speculum shall have a Rockwell hardness of C-40 to C-45 when tested for hardness in accordance with ASTM E18 or ASTM E92 and E140.

Style and design. The speculum shall be a nasal speculum with a screw pivot and thin 2 inch blades. Removal of the screw shall facilitate separation of the blades for repair and cleaning. The speculum shall be capable of easy opening when normal hand pressure is applied and shall close freely without binding or setting when the pressure is released. The style and dimensions shall be in accordance with Figure 1.

Finish. The finish shall be satin and mirror or mirror in accordance with Federal Specification GG-I-526.

Passivation. The speculum shall be properly passivated.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Markings. The speculum shall be marked with the name or registered trademark of the contractor. The speculum shall have the word "stainless" marked on the instrument. If the speculum is of foreign manufacture, the instrument shall be marked with the country of origin.

Corrosion resistance. The speculum shall show no evidence of corrosion or plating of copper sulfate when tested in accordance with the Copper Sulfate and Boil Tests of Federal Specification GG-I-526.

Blade operation. The speculum shall be opened and closed 5 times. The blades shall meet. The speculum shall open and close freely without binding or sticking.

Workmanship. The speculum shall be free from defects which detract from its appearance or impair its serviceability.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One speculum, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:59Z
Check the source to verify that this is the currentversion before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for visual examination shall be in accordance with MIL-STD-105. The unit of product for examination shall be one speculum. Sampling shall be Level II with an AQL of 6.5.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one speculum. AQL shall be 1.0 percent defective. Inspection level shall be S-2.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric Products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-113-2629	SPECULUM, SEPTUM, COTTLE

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51702A

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4024

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:59Z
Check the source to verify that this is the current version before use.

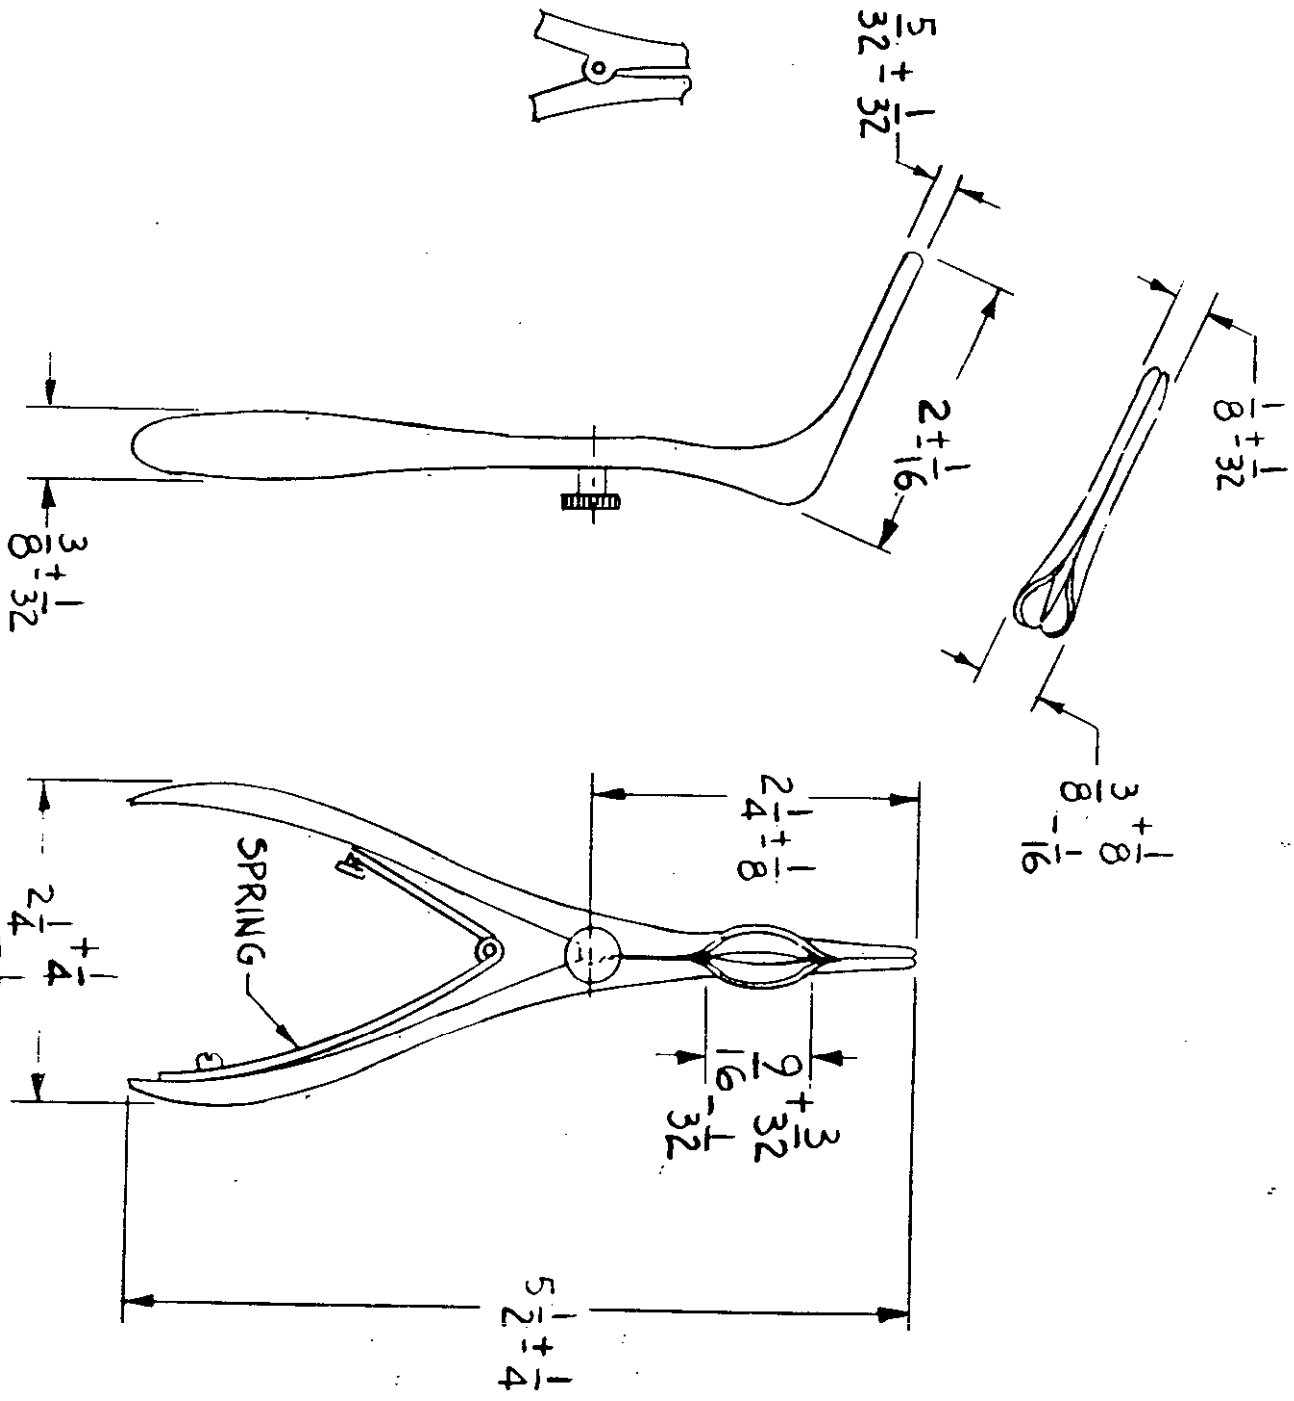


FIGURE 1 SPECULUM, SEPTUM, COTTLE

NOTE: ALL DIMENSIONS ARE IN INCHES

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:59Z
Check the source to verify that this is the current version before use.